

**Riverside County Fire Department**  
**Perris, CA**  
**Air/Light- SVI #1254**  
**Production Specification**



## **LIABILITY INSURANCE**

The manufacturer shall furnish with the bid a certificate of insurance for;

Workman's Compensation and Employer's Liability Insurance covering for all employees.

General Liability (each occurrence) of \$1,000,000.00. General Aggregate coverage of \$2,000,000.00. Products Completed / Operations Aggregate coverage of \$2,000,000.00. Medical Expense coverage of \$5,000 (any one person). Personal Injury of \$1,000,000.00.

Automobile liability of \$1,000,000.00 combined single limit (each accident), including any auto, all owned autos, scheduled autos, hired autos, non-owned autos, and garage liability.

Excess Umbrella Liability coverage of \$6,000,000.00 each occurrence, Aggregate of \$6,000,000.00. Garage Keepers Liability coverage of \$6,000,000.00 combined limit.

All insurance policies must be;

- Maintained for the life of the contract,
- Must provide ten (10) days notice before cancellation,
- Must cover all operations of the contractor, or anyone employed by them.

## **INTERNET IN-PROCESS SITE**

The manufacturer shall post and maintain a website where the Riverside County Fire Department will be able to view digital images of their apparatus as its being built. The digital images shall be posted once a week starting when the body begins production or when the cab/chassis arrives and shall continue until the final completion of unit.

## **RESPONSIBILITY OF PURCHASER**

It shall be the responsibility of the purchaser to specify the details of the apparatus in addition to the requirements in NFPA 1901 needed by the manufacturer to build the apparatus, including:

- 1) Requirements not uniquely specified in NFPA 1901, such as the type of apparatus desired.
- 2) Any features of the apparatus desired in addition to, or in excess of, the requirements in NFPA 1901.

After acceptance of the fire apparatus, the purchaser shall be responsible for ongoing training of personnel to develop and maintain proficiency regarding the proper and safe use of the apparatus and the associated equipment.

## **RESPONSIBILITY OF CONTRACTOR**

The Contractor shall provide a detailed description of the apparatus, a list of equipment to be furnished, and other construction and performance details to which the apparatus shall conform. The detailed description of the apparatus shall include, but shall not be limited to,

1. Estimated In-Service Weight,
2. Wheelbase, Turning Clearance Radius,
3. Principal dimensions, Angle of Approach, Angle of Departure,
4. Transmission, Axle Ratios.

The Contractor's detailed description shall include a statement specifically describing each aspect of the delivered apparatus that will not be fully compliant with the requirements of this standard.

The purpose of these Contractor specifications shall be to define what the contractor intends to furnish and deliver to the purchaser.

Responsibility for the apparatus and equipment shall remain with the contractor until they are accepted by the purchaser.

### **VEHICLE STABILITY SUPPLIED WITH CAB/CHASSIS**

The cab/chassis shall be equipped with a stability control system. The system shall have, at a minimum, a steering wheel position sensor, a vehicle yaw sensor, a lateral accelerometer and individual wheel brake controls.

### **FIRE APPARATUS PERFORMANCE**

The fire apparatus shall meet the requirements of this standard at elevations of 2000 ft (600 m) above sea level.

The fire apparatus shall meet all the requirements of this standard while stationary on a grade of 6 percent in any direction.

The fire apparatus shall meet the requirements of this standard in ambient temperature conditions between 32°F (0°C) and 110°F (43°C).

### **HIGHWAY PERFORMANCE**

The apparatus, when loaded to its estimated in-service weight, shall be capable of the following performance while on dry, paved roads that are in good condition:

- 1) Accelerating from 0 to 35 mph (55 km/hr) within 25 seconds on a 0 percent grade
- 2) Attaining a speed of 50 mph (80 km/hr) on a 0 percent grade
- 3) Maintaining a speed of at least 20 mph (32 km/hr) on any grade up to and including 6 percent

The maximum top speed of fire apparatus with a GVWR over 26,000 lb (11,800 kg) shall not exceed either 68 mph (109 km/hr) or the manufacturer's maximum fire service speed rating for the tires installed on the apparatus, whichever is lower.

If the combined water tank and foam agent tank capacities on the fire apparatus exceed 1250 gal (4732 L), or the GVWR of the vehicle is over 50,000 lb (22,680 kg), the maximum top speed of the apparatus shall not exceed either 60 mph (95 km/hr) or the manufacturer's maximum fire service speed rating for the tires installed on the apparatus, whichever is lower.

### **SERVICEABILITY**

The fire apparatus shall be designed to allow the manufacturer's recommended routine maintenance checks of lubricant and fluid levels to be performed by the operator without lifting the cab of a tilt-cab apparatus or without the need for hand tools.

Where special tools are required for routine service on any component of the apparatus, such tools shall be provided with the apparatus.

Apparatus components that interfere with repair or removal of other major components shall be attached with fasteners, such as cap screws and nuts, so that the components can be removed and installed with ordinary hand tools. These components shall not be welded or otherwise permanently secured into place.

## **FIRE APPARATUS DOCUMENTATION**

The contractor shall supply, at the time of delivery, at least one (1) copy of the following documents:

- 1) The manufacturers record of apparatus construction details, including the following documents:
  - a) Owner's name and address
  - b) Apparatus manufacturer, model, and serial number
  - c) Chassis make, model, and serial number
  - d) GAWR of front and rear axles and GVWR
  - e) Front tire size and total rated capacity in pounds (kilograms)
  - f) Rear tire size and total rated capacity in pounds (kilograms)
  - g) Chassis weight distribution in pounds (kilograms) with water and manufacturer-mounted equipment (front and rear)
  - h) Engine make, model, serial number, rated horsepower and related speed, and governed speed; and if so equipped, engine transmission PTO(s) make, model, and gear ratio
  - i) Type of fuel and fuel tank capacity
  - j) Electrical system voltage and alternator output in amps
  - k) Battery make, model, and capacity in cold cranking amps (CCA)
  - l) Chassis transmission make, model, and serial number; and if so equipped, chassis transmission PTO(s) make, model, and gear ratio
  - m) Ratios of all driving axles
  - n) Maximum governed road speed
  - o) Pump make, model, rated capacity in gallons per minute (liters per minute where applicable), maximum discharge pressure capability rating, and serial number
  - p) Pump transmission make, model, serial number, and gear ratio
  - q) Auxiliary pump make, model, rated capacity in gallons per minute (liters per minute where applicable), and serial number
  - r) Water tank certified capacity in gallons or liters
  - s) Foam tank (if provided) certified capacity in gallons (liters)
  - t) Aerial device type, rated vertical height in feet (meters), rated horizontal reach in feet (meters), and rated capacity in pounds (kilograms)
  - u) Paint manufacturer and paint number(s)
  - v) Company name and signature of responsible company representative
  - w) Weight documents from a certified scale showing actual loading on the front axle, rear axle(s), and overall fire apparatus (with the water tank full but without personnel, equipment, and hose)
- 2) Certification of compliance of the optical warning system (*see 13.8.16*)
- 3) Siren manufacturer's certification of the siren (*see 13.9.1.1*)
- 4) Written load analysis and results of the electrical system performance tests (*see 13.14.1 and Section 13.15*)
- 5) Certification of slip resistance of all stepping, standing, and walking surfaces (*see 15.7.4.5*)
- 6) If the apparatus has a fire pump, the pump manufacturer's certification of suction capability (*see 16.2.4.1*)
- 7) If the apparatus is equipped with a fire pump and special conditions are specified by the purchaser, the pump manufacturer's certification of suction capacity under the special conditions (*see 16.2.4.2*)
- 8) If the apparatus has a fire pump, a copy of the apparatus manufacturer's approval for stationary pumping applications (*see 16.3.1*)
- 9) If the apparatus has a fire pump, the engine manufacturer's certified brake horsepower curve for the engine furnished, showing the maximum governed speed (*see 16.3.2.2*)
- 10) If the apparatus has a fire pump, the pump manufacturer's certification of the hydrostatic test (*see 16.5.2.2*)
- 11) If the apparatus has a fire pump with a maximum discharge pressure capability rating that exceeds the hydrostatic test pressure of 16.5.2.1, the pump manufacturer's certification of the hydrodynamic test

- 12) If the apparatus has a fire pump, the certification of inspection and test for the fire pump (*see 16.13.1.1.5 or 16.13.1.2.4 as applicable*)
- 13) If the apparatus is equipped with an auxiliary pump, the apparatus manufacturer's certification of the hydrostatic test (*see Section 17.13*)
- 14) When the apparatus is equipped with a water tank, the certification of water tank capacity (*see Section 18.6*)
- 15) If the apparatus has an aerial device, the certification of inspection and test for the aerial device (*see Section 19.24*)
- 16) If the apparatus has an aerial device, all the technical information required for inspections to comply with NFPA 1911
- 17) If the apparatus has a foam proportioning system, the foam proportioning system manufacturer's certification of accuracy (*see 20.10.4.2*) and the final installer's certification the foam proportioning system meets this standard (*see 20.11.2*)
- 18) If the system has a CAFS, the documentation of the manufacturer's pre delivery tests (*see Section 21.9*)
- 19) If the apparatus has a line voltage power source, the certification of the test for the power source (*see 22.15.7.2*)
- 20) If the apparatus is equipped with an air system, air tank certificates (*see 24.5.1.2*), the SCBA fill station certification (*see 24.9.6*), and the results of the testing of the air system installation (*see 24.14.5 and 24.15.4*)
- 21) Any other required manufacturer test data or reports

## **OPERATIONS AND SERVICE DOCUMENTATION**

The contractor shall deliver with the fire apparatus complete operation and service documentation covering the completed apparatus as delivered and accepted.

The documentation shall address at least the inspection, service, and operations of the fire apparatus and all major components thereof.

The contractor shall also deliver with the fire apparatus the following documentation for the entire apparatus and each major operating system or major component of the apparatus:

- 1) Manufacturer's name and address
- 2) Country of manufacture
- 3) Source for service and technical information
- 4) Parts replacement information
- 5) Descriptions, specifications, and ratings of the chassis, pump (if applicable), and aerial device (if applicable)
- 6) Wiring diagrams for low voltage and line voltage systems to include the following information:
  - a) Pictorial representations of circuit logic for all electrical components and wiring
  - b) Circuit identification
  - c) Connector pin identification
  - d) Zone location of electrical components
  - e) Safety interlocks
  - f) Alternator–battery power distribution circuits
  - g) Input/output assignment sheets or equivalent circuit logic implemented in multiplexing systems
- 7) Lubrication charts
- 8) Operating instructions for the chassis, any major components such as a pump or aerial device, and any auxiliary systems
- 9) Precautions related to multiple configurations of aerial devices, if applicable
- 10) Instructions regarding the frequency and procedure for recommended maintenance
- 11) Overall apparatus operating instructions
- 12) Safety considerations
- 13) Limitations of use
- 14) Inspection procedures
- 15) Recommended service procedures
- 16) Troubleshooting guide
- 17) Apparatus body, chassis and other component manufacturer's warranties

- 18) Special data required by this standard
- 19) A material safety data sheet (MSDS) for any fluid that is specified for use on the apparatus

The contractor shall deliver with the apparatus all manufacturer's operations and service documents supplied with components and equipment that are installed or supplied by the contractor.

#### **NFPA REQUIRED DOCUMENTATION FORMAT - USB FLASH DRIVE**

The vehicle construction details and the operations and service documentation as required per NFPA 1901 latest edition shall be provided on a USB Flash Drive. These manuals shall be divided into sections for ease of reference. There shall be two (2) USB flash drives provided with the completed vehicle.

#### **FIRE APPARATUS SAFETY GUIDE**

A Fire Apparatus Safety Guide published by Fire Apparatus manufacturer's Association shall be provided with delivered vehicle. This manual includes essential safety information for fire fighters, fire chiefs, apparatus mechanics, and fire department safety officers. The guide is applicable to municipal, wildland, and airport fire fighting apparatus manufactured on either custom or commercial chassis.

#### **STATEMENT OF EXCEPTIONS**

The final-stage manufacturer shall deliver with the fire apparatus either a certification that the apparatus fully complies with all requirements of this standard or alternatively, a Statement of Exceptions specifically describing each aspect of the completed apparatus that is not fully compliant with the requirements of this standard at the time of delivery.

The Statement of Exceptions shall contain, for each noncompliant aspect of the apparatus or missing required item, the following information:

- 1) A separate specification of the section of the applicable standard for which compliance is lacking
- 2) A description of the particular aspect of the apparatus that is not in compliance therewith or required equipment that is missing
- 3) A description of the further changes or modifications to the delivered apparatus that must be completed to achieve full compliance
- 4) Identification of the entity that will be responsible for making the necessary post delivery changes or modifications or for supplying and installing any missing required equipment to the apparatus to achieve full compliance with this standard

Prior to or at the time of delivery of the apparatus, the Statement of Exceptions shall be signed by an authorized agent of the entity responsible for final assembly of the apparatus and by an authorized agent of the purchasing entity, indicating mutual understanding and agreement between the parties regarding the substance thereof.

#### **CARRYING CAPACITY**

The GAWR and the GCWR or GVWR of the chassis shall be adequate to carry the weight of the completed vehicle when loaded to its estimated in-service weight. The manufacturer shall establish the estimated in service weight during the design of the vehicle.

The estimated in-service weight shall include the following:

1. The chassis, body and tank(s)
2. Full fuel, lubricant, and other chassis or component fluid tanks or reservoirs
3. Full water and other agent tanks

4. \*250 lb (114 kg) in each seating position
5. Fixed equipment such as pumps, aerial devices, generators, reels and air systems as installed
6. Ground ladders, suction hose, designed hose load in their hose beds and on their reels
7. An allowance for miscellaneous equipment that is the greatest of the following:
  - a) The values shown for items 1 - 7
  - b) A purchaser-provided list of equipment to be carried with weights
  - c) A purchaser-specified miscellaneous equipment allowance

The manufacturer shall engineer and design the fire apparatus such that the completed apparatus, when loaded to its estimated in-service weight, with all movable weights distributed as close as is practical to their intended in-service configuration, does not exceed the GVWR.

A final manufacturer's certification of the GVWR or GCWR, along with a certification of each GAWR, shall be supplied on a label affixed to the vehicle.

The fire apparatus manufacturer shall permanently affix a high-visibility label in a location visible to the driver while seated.

The label shall show the height of the completed unequipped fire apparatus in feet and inches (meters), the length of the completed fire apparatus in feet and inches (meters), and the GVWR in tons (metric tons).

Wording on the label shall indicate that the information shown was current when the apparatus was manufactured and that, if the overall height changes while the vehicle is in service, the fire department must revise that dimension on the plate.

<b>Apparatus Type</b>	<b>Equip. Storage Area</b>	<b>Apparatus Size</b>	<b>Equipment Allowance</b>	
			<b>lb.</b>	<b>kg.</b>
Special Service Fire Apparatus	Minimum of 120 cu ft (3.4 cu mt) of enclosed compartmentation.	10,000 lb to 15,000 lb (4,500 kg to 7,000 kg) GVWR	2,000	910
		15,001 lb to 20,000 lb (7,001 kg to 9,000 kg) GVWR	2,500	1,135
		20,001 lb to 30,000 lb (9,001 kg to 14,000 kg) GVWR	3,000	1,350
		30,001 lb to 40,000 lb (14,001 kg to 18,000 kg) GVWR	4,000	1,800
		40,001 lb to 50,000 lb (18,001 kg to 23,000 kg) GVWR	6,000	2,700
		50,001 lb to 60,000 lb (23,001 kg to 27,000 kg) GVWR	8,000	3,600
		60,001 lb and up (27,001 kg) GVWR	10,000	4,500

## **TESTING**

### **ROAD TEST**

Each apparatus shall be tested by the manufacturer before delivery to verify that it meets the following criteria;

Tests shall be conducted at a location and in a manner that does not violate local, state or provincial, or federal traffic laws. Tests shall be conducted on a dry, level, paved surface that is free of loose material, oil, or grease. Tests shall be conducted with the water and foam tanks full (water or product).

The apparatus shall accelerate from 0 to 35 mph (55 km/hr) within 25 seconds. The apparatus shall attain a speed of 50 mph (80 km/hr).

The auxiliary braking system, if so equipped, shall function as intended by the auxiliary braking system manufacturer.

The air service brakes shall bring the apparatus to a complete stop from a speed of 20 mph (32.2 km/hr) in a distance not exceeding 35 ft (10.7 m).

The hydraulic service brakes shall bring the apparatus to a complete stop from a speed of 30 mph (48.2 km/hr) in a distance not exceeding 88 ft (26.8 m).

### **LOW VOLTAGE - ELECTRICAL SYSTEM PERFORMANCE TEST**

The vehicles low voltage electrical system shall be tested and certified by the manufacturer. The certified test results shall be delivered with the completed vehicle. Tests shall be performed when the air temperature is between 0°F and 110°F (–18°C and 43°C).

### **TEST SEQUENCE**

The following three (3) tests shall be performed in the order in which they appear below. Before each test, the batteries shall be fully charged until the voltage stabilizes at the voltage regulator set point and the lowest charge current is maintained for ten (10) minutes. Failure of any of these tests shall require a repeat of the sequence.

#### **1. RESERVE CAPACITY TEST**

The engine shall be started and kept running until the engine and engine compartment temperatures are stabilized at normal operating temperatures and the battery system is fully charged. The engine shall be shut off and the minimum continuous electrical load shall be activated for ten (10) minutes.

All electrical loads shall be turned off prior to attempting to restart the engine. The battery system shall then be capable of restarting the engine. Failure to restart the engine shall be considered a test failure of the battery system.

#### **2. ALTERNATOR PERFORMANCE TEST**

##### **TEST AT IDLE**

The minimum continuous electrical load shall be activated with the engine running at idle speed. The engine temperature shall be stabilized at normal operating temperature. The battery system shall be tested to detect the presence of battery discharge current. The detection of battery discharge current shall be considered a test failure.

##### **TEST AT FULL LOAD**



The total continuous electrical load shall be activated with the engine running up to the engine manufacturer's governed speed. The test duration shall be a minimum of two (2) hours. Activation of the load management system shall be permitted during this test.

An alarm sounded by excessive battery discharge, as detected by the warning system required in 13.3.4, or a system voltage of less than 11.8 V dc for a 12 V nominal system, 23.6 V dc for a 24 V nominal system, or 35.4 V dc for a 42 V nominal system for more than 120 seconds shall be considered a test failure.

### **3. LOW VOLTAGE ALARM TEST**

The following test shall be started with the engine off and the battery voltage at or above 12 V for a 12 V nominal system, 24 V for a 24 V nominal system or 36 V for a 42 V nominal system.

With the engine shut off, the total continuous electrical load shall be activated and shall continue to be applied until the excessive battery discharge alarm activates. The battery voltage shall be measured at the battery terminals.

The test shall be considered a failure if the alarm does not sound in less than 140 seconds after the voltage drops to 11.70 V for a 12 V nominal system, 23.4 V dc for a 24 V nominal system, or 35.1 V for a 42 V nominal system.

The battery system shall then be able to restart the engine. Failure to restart the engine shall be considered a test failure.

### **LOW VOLTAGE - ELECTRICAL SYSTEM PERFORMANCE TEST**

#### **DOCUMENTATION**

The manufacturer shall deliver the following with the fire apparatus:

- 1) Documentation of the electrical system performance tests
- 2) A written electrical load analysis, including the following:
  - a) The nameplate rating of the alternator
  - b) The alternator rating
  - c) Each of the component loads specified that make up the minimum continuous electrical load
  - d) Additional electrical loads that, when added to the minimum continuous electrical load, determine the total continuous electrical load
  - e) Each individual intermittent electrical load

### **UL 120/240 VAC CERTIFICATION**

The 120/240 volt electrical system shall be third-party, independent, audit-certified through Underwriters Laboratory (UL) to the current edition of NFPA 1901 to perform as listed below;

The prime mover shall be started from a cold start condition, and the unloaded voltage and frequency shall be recorded.

The line voltage electrical system shall be loaded to at least 100% of the continuous rated wattage stated on the power source specification label. Testing with a resistive load bank shall be permitted.

The power source shall be operated in the manner specified by the apparatus manufacturer as documented on instruction plates or in operation manuals. The power source shall be operated at a minimum of 100% of the continuous rated wattage as stated on the power source specification label for a minimum of two (2) hours.

The load shall be adjusted to maintain the output wattage at or above the continuous rated wattage during the entire 2-hour test.

The following conditions shall be recorded at least every 1/2 hour during the test:

- 1) The power source output voltage, frequency and amperes
- 2) The prime mover's oil pressure, water temperature and transmission temperature, if applicable
- 3) The power source hydraulic fluid temperature, if applicable
- 4) The ambient temperature and power source air inlet temperature

The following conditions shall be recorded once during the test for power sources driven by dedicated auxiliary internal combustion engines:

- 1) Altitude
- 2) Barometric pressure
- 3) Relative humidity

If the generator is driven by the chassis engine and the generator allows for operation at variable speeds, the chassis engine speed shall be reduced to the lowest rpm allowed for generator operation and the voltage and frequency shall be recorded.

The load shall be removed and the unloaded voltage and frequency shall be recorded.

Voltage shall be maintained within  $\pm 10\%$  of the voltage stated on the power source specification label during the entire test. Frequency shall be maintained within  $\pm 3$  Hz of the frequency stated on the power source specification label during the entire test.

The total continuous electrical loads, excluding those loads associated with the equipment defined in NFPA 22.15.7.3.11.2, shall be applied during the testing unless an auxiliary engine drives the power source.

If the apparatus is equipped with a fire pump, the 2-hour certification test of the power source shall be completed with the fire pump pumping at 100% capacity at 150 psi (1000 kPa) net pump pressure. The test shall be permitted to be run concurrently with the pump certification test.

## **DOCUMENTATION**

The results of each test shall be recorded on an appropriate form and provided with the delivery of the fire apparatus.

## **DIELECTRIC VOLTAGE WITHSTAND TEST**

The line voltage wiring and permanently connected devices and equipment shall be subjected to a dielectric voltage withstand test of 900 volts for one (1) minute. The testing shall be performed after all body work has been completed.

The test shall be conducted as follows:

- 1) Isolate the power source from the panel board and disconnect any solid state low voltage components
- 2) Connect one lead of the dielectric tester to all the hot and neutral buses tied together
- 3) Connect the other lead to the fire apparatus frame or body
- 4) Close any switches and circuit breakers in the circuit(s)
- 5) Apply the dielectric voltage for one (1) minute in accordance with the testing equipment manufacturer's instructions

The electrical polarity of all permanently wired equipment, cord reels and receptacles shall be tested to verify that wiring connections have been properly made.

Electrical continuity shall be verified from the chassis or body to all line voltage electrical enclosures, light housings, motor housings, light poles, switch boxes and receptacle ground connections that are accessible to fire fighters in normal operations.

If the apparatus is equipped with a transfer switch, it shall be tested to verify operation and that all non grounded conductors are switched.

Electrical light towers, floodlights, motors, fixed appliances and portable generators shall be operated at their full rating or capacity for 30 minutes to ensure proper operation.

## **WARRANTY**

A full statement shall be provided of the warranties for the vehicle(s) being bid. Warranties should clearly describe the terms under which the vehicle manufacturer accepts responsibility for the cost to repair defects caused by faulty design, quality of work or material and for the applicable period of time after delivery.

Cost of repairs refers to all costs related thereto including, but not limited to, the cost of materials and the cost of labor.

The Body Manufacturer shall warrant all materials and accessories used on the vehicle(s), whether fabricated by manufacturer or purchased from an outside source and will deal directly with the Riverside County Fire Department on all warranty work.

### **GENERAL LIMITED WARRANTY - TWO (2) YEARS**

The vehicle shall be free of defects in material and workmanship for a period of two (2) years or 36,000 miles (or 57,936 kilometers), whichever occurs first starting thirty (30) days after the original invoice date.

The Contractor must be the "single source" coordinator of all warranties on the vehicle.

### **LOW VOLTAGE ELECTRICAL WARRANTY - FIVE (5) YEARS**

The vehicle low voltage electrical system shall be free of defects in material and workmanship for a period of five (5) years or 60,000 miles (or 96,561 kilometers), whichever occurs first, starting thirty (30) days after the original invoice date.

### **STRUCTURAL WARRANTY - TEN (10) YEARS**

The body shall be free of structural or design failure or workmanship for a period of ten (10) years, or 100,000 miles (or 160,934 kilometers), whichever occurs first, starting thirty (30) days after the original invoice date.

### **UNDERCOAT WARRANTY**

The body undercoating shall have a warranty provided by the manufacturer for the lifetime of the vehicle or twenty (20) years, whichever occurs first. The warranty shall be transferable between vehicle owners. Should the undercoating material applied to the underside of the body and wheel wells of the vehicle ever flake off, peel, chip or crack due to drying out, the damaged area shall be re-sprayed without charge to the vehicle owner.

### **PAINT LIMITED WARRANTY - TEN (10) YEARS**

The body shall be free of bubbling or peeling as a result of a defect in the method of manufacture for a period of ten (10) years or 100,000 miles (or 160,934 kilometers), whichever occurs first, starting thirty (30) days after the original invoice date. **Pro-rated warranties will not be acceptable.**

### **GRAPHICS LIMITED WARRANTY**

The 3M graphics installation shall be warranted for a period of two (2) years. The 3M materials installed on completed vehicle shall be warranted for seven (7) years. The 3M Diamond grade film (if specified) shall be warranted for ten (10) years.

### **CONSTRUCTION PERIOD**

The completed vehicle shall be delivered within five hundred ninety (590) days after pre-construction meeting and receipt and approval of any signed change orders from Riverside County Fire Department.

Contractor shall not be held liable for delays of chassis delivery due to accidents, strikes, floods or other events not subject to their control. Contractor shall provide written notice to Riverside County Fire Department as to delays and to what extent these delays have in completing vehicle within the stated construction time period.

### **OVERALL HEIGHT REQUIREMENT**

There is no overall height (OAH) restriction for this vehicle.

### **OVERALL LENGTH REQUIREMENT**

There is no overall length (OAL) restriction for this vehicle.

### **ANGLE OF APPROACH**

The angle of approach for this vehicle shall not be less than eight (8) degrees when it is loaded to the estimated in-service weight as specified by the current edition of NFPA 1901.

### **ANGLE OF DEPARTURE**

The angle of departure for this vehicle shall not be less than eight (8) degrees when it is loaded to the estimated in-service weight as specified by the current edition of NFPA 1901.

Inspection Trips, Delivery, Demonstration

### **PRE-CONSTRUCTION CONFERENCE**

A pre-construction conference shall be required at the Contractor's factory for two (2) personnel from the Riverside County Fire Department to finalize all construction details prior to manufacturing.

The Contractor shall at his/her expense, provide transportation, lodging, rental car and meal expenses during the pre-construction conference. Any travel distance greater than 250 miles shall be by non-stop commercial air travel.

### **PRE-PAINT CONFERENCE**

A pre-paint conference shall be required at the Contractor's factory for one (1) personnel from the Riverside County Fire Department to inspect the vehicle and construction details prior to the painting process.

The Contractor shall at his/her expense, provide transportation, lodging, rental car and meal expenses during the pre-paint conference. Any travel distance greater than 250 miles shall be by non-stop commercial air travel.

## **FINAL INSPECTION CONFERENCE**

A final inspection conference shall be required at the Contractor's factory for two (2) personnel from the Riverside County Fire Department to inspect the vehicle and construction details prior to shipment of the completed vehicle. This inspection shall take place after any specified striping and lettering is installed.

The Contractor shall at his/her expense, provide transportation, lodging, rental car and meal expenses during the final inspection conference. Any travel distance greater than 250 miles shall be by non-stop commercial air travel.

## **DELIVERY AND DEMONSTRATION**

The Contractor shall be responsible for the delivery of the completed unit to the Riverside County Fire Department's location. On initial delivery of the apparatus, the Contractor shall supply a qualified representative to demonstrate the apparatus and provide initial instruction to representatives of the Riverside County Fire Department regarding the operation, care and maintenance of the apparatus and equipment supplied at Riverside County Fire Department location.

The Delivery Engineer shall set delivery and instruction schedule with the person appointed by Riverside County Fire Department.

After delivery of the apparatus, the Riverside County Fire Department shall be responsible for ongoing training of its personnel to proficiency regarding the proper and safe use of the apparatus and associated equipment.

## **SPARTAN ER SUPPLIED CHASSIS**

### **CAB TO AXLE DIMENSION**

Cab to axle will be 126.5".

### **FRONT BUMPER**

The front bumper shall be provided by the cab/chassis manufacturer.

### **BUMPER GRAVELSHIELD**

The bumper extension gravel shield if specified shall be provided by the cab/chassis manufacturer.

### **FRONT TOW PROVISIONS**

The front tow provisions if specified shall be supplied and installed by the cab/chassis manufacturer.

### **SIREN SPEAKER**

The siren speaker(s) shall be supplied and installed by the cab/chassis manufacturer.

### **AIR INTAKE SYSTEM**

An air filter shall be provided in the engine's air intake system by the customer cab/chassis manufacturer.

Air inlet restrictions shall not exceed the engine manufacturer's recommendations.

The air inlet shall be equipped with a means of separating water and burning embers from the air intake system.

This requirement shall be permitted to be achieved by either of the following methods:

1. Provision of a device such that burning particulate matter larger than 0.039 in. (1.0 mm) in diameter cannot reach the air filter element.
2. Provision of a multi screen ember separator capable of meeting the test requirements defined in the Parker Hannafin, Racor Division, publication LF 1093-90, *Ember Separation Test Procedure*, or an equivalent test.

### **EXHAUST DIVERTER**

An exhaust diverter valve shall be located in-line of exhaust tubing and controlled from driver's position to re-route exhaust discharge. Exhaust diverter valve shall be constructed from 14 gauge stainless steel material with air actuated control.

As a default, the exhaust shall always discharge to curbside just ahead of rear wheels, and when selected the exhaust shall discharge to a vertical exhaust pipe, extending above the body height 12".

The exhaust piping and discharge outlet shall be located or shielded so as not to expose any portion of the apparatus or equipment to excessive heating.

Exhaust pipe discharge shall be directed away from any operator's position.

Where parts of the exhaust system are exposed so that they are likely to cause injury to operating personnel, protective guards shall be provided.

- Exhaust Diverter shall be controlled by a momentary rocker switch with red actuator and red Indicator. Rocker Switch will be located in the center console/dash panel and shall be labeled "EXHAUST DIVERTER".

### **PLYMOVENT EXHAUST ADAPTER**

A Plymovent 5" exhaust adapter flange for Plymovent pneumatic systems shall be provided and installed on the chassis engine exhaust tailpipe.

**SVI Install of chassis Supplied Plymovent and Add a stopper plate at 3".**

- The tail pipe(s) shall terminate parallel to rear axle and flush with body.

### **WARNING LIGHT: CHASSIS CAB**

Warning Lights: Chassis Cab, Custom, Whelen

### **ZONE A - FRONT WARNING LIGHTS, UPPER**

The light bar shall be supplied and installed by the cab/chassis manufacturer.

The lightbar(s) shall be separately controlled at multiplex display(s) in the cab.

### **GTT OPTICOM**

A GTT Opticom model 792H Infrared emitter strobe style light with built-in power supply shall be provided as a stand alone unit (outside of light bar).

- Opticom shall be controlled by a virtual switch, labeled "OPTICOM", and interlocked with the parking brake (transmission park position) same as other clear warning.

#### ZONE A - FRONT WARNING LIGHTS, LOWER

The warning lights shall be supplied and installed by the cab/chassis manufacturer. They shall be Whelen lights to complete an NFPA compliant lower level warning light system.

The lights shall be controlled at the multiplex display(s) in the cab.

#### ZONES B AND D - CAB INTERSECTOR LIGHT (CAB FRONT CORNERS)

The warning lights shall be supplied and installed by the cab/chassis manufacturer. They shall be Whelen lights to complete an NFPA compliant lower level warning light system.

The lights shall be controlled at the multiplex display(s) in the cab.

#### CAB HAZARD WARNING LIGHT - EXHAUST DIVERTER

A Truck-Lite amber LED flashing light shall be provided and located in the driving compartment and be illuminated automatically whenever the vehicles exhaust diverter is active

The hazard light shall be labeled; "Do not move apparatus when light is on."

#### RUMBLER PROGRAMMING

The cab/chassis supplied **Rumbler shall be programmed by SVI as follows:**

**Rumbler Activation:** The chassis supplied Rumbles will need to be linked with the siren head at SVI so that the Rumbles are active when the siren head is set to Wail or Yelp. They shall then activate with the steering wheel activation or the chassis supplied/installed siren button on the officer side.

#### FIVE (5) POSITION ANTENNA RAIL

One (1) radio antenna rail(s) shall be provided and installed on roof of vehicle. Each rail be constructed of aluminum, forming a two piece box design. The top section shall be removable for easy access to the individual antenna wiring. Each base shall include enough cable to reach radio location plus a service loop of at least 10' of LMR195 flexible communications cable. The antenna wiring shall enter the vehicle roof at a single point under the end of the rail.

**Conduit with cable pull wire shall be installed from the Antenne Rail to behind the officer seat position**

**Antenna #1 chassis supplied AM/FM Antennae mounted on specified antenna rail.**

Due to multiple configurations of antenna whips, the Body Manufacturer shall provide the antenna base, and Riverside County Fire Department shall provide the whip.

The end of antenna cable shall be routed to overhead driver area. Cable shall be labeled for **PROVIDE INFORMATION.**

Antenna #2 mounted and installed on specified antenna rail.

Due to multiple configurations of antenna whips, the Body Manufacturer shall provide the antenna base, and Riverside County Fire Department shall provide the whip.

The end of antenna cable shall be routed to center dash. Cable shall be labeled for **PROVIDE INFORMATION**.

Antenna #3 mounted and installed on specified antenna rail.

Due to multiple configurations of antenna whips, the Body Manufacturer shall provide the antenna base, and Riverside County Fire Department shall provide the whip.

The end of antenna cable shall be routed to center dash. Cable shall be labeled for **PROVIDE INFORMATION**.

Antenna #4 mounted and installed on specified antenna rail.

Due to multiple configurations of antenna whips, the Body Manufacturer shall provide the antenna base, and Riverside County Fire Department shall provide the whip.

The end of antenna cable shall be routed to center dash. Cable shall be labeled for **PROVIDE INFORMATION**.

Antenna #5 mounted and installed on specified antenna rail.

Due to multiple configurations of antenna whips, the Body Manufacturer shall provide the antenna base, and Riverside County Fire Department shall provide the whip.

The end of antenna cable shall be routed to center dash. Cable shall be labeled for **PROVIDE INFORMATION**.

Antenna rail will be painted to match the exterior color of the chassis.

Cab roof mounted antenna rail shall be located on rear roof section.

### **SEAT BELT COLOR**

Section 14.1.3.3 of the NFPA 1901 Standards, requires all seat belt webbing in cab to be bright red or bright orange in color, and the buckle portion of the seat belt shall be mounted on a rigid or semi rigid stalk such that the buckle remains positioned in an accessible location.

### **SEAT BELT WEB LENGTH - CUSTOM CAB**

Sections 14.1.3.2 and 14.1.3.3 of the NFPA 1901 standards, require the effective seat belt web length for a Type 1 lap belt for pelvic restraint to be a minimum of 60", and a Type 2 pelvic and upper torso restraint-style seat belt assembly to be a minimum of 110".

The chassis seat belt web length as supplied by the custom chassis manufacturer shall be compliant to NFPA Standards 14.1.3.2 and 14.1.3.3.


### **SEAT BELT / VDR SYSTEM - CUSTOM CAB**

The seat belt warning and vehicle data recorder systems shall be provided by the cab/chassis manufacturer.



## **CAB CONSOLE**

A custom console shall be provided to match:

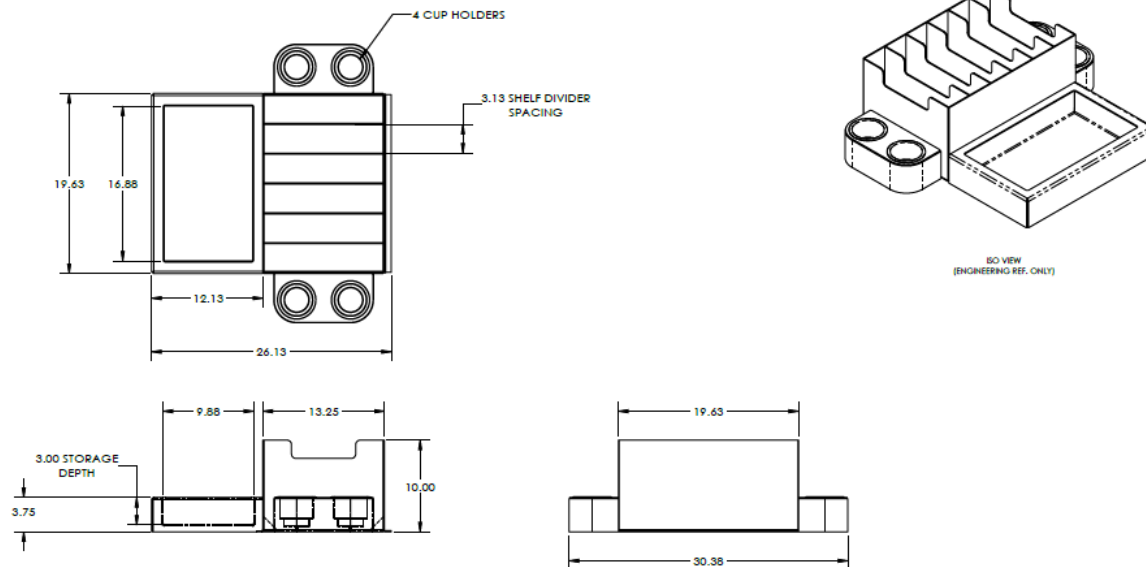

## **TIRE PRESSURE VISUAL INDICATORS**

Tire pressure visual indicators if specified shall be supplied by the cab and chassis manufacturer.

## **HELMET STORAGE, DRIVING AREA**

No helmet storage is required in the cab driving area. A safety sign FAMA15, which warns not to wear helmets while the vehicle is in motion, shall be visible from each seat that is intended to be occupied while the vehicle is in motion.

## **HELMET STORAGE, CREW AREA**

No helmet storage is required in the cab crew area. A safety sign FAMA15, which warns not to wear helmets while the vehicle is in motion, shall be visible from each seat that is intended to be occupied while the vehicle is in motion.

## **CAB CRASH TEST CERTIFICATION**

A cab crash test certification from the fire apparatus manufacturer shall be provided with the equipment. A copy of this certification shall be included with the bid.

NOTE: There shall be no exception to any portion of the cab integrity certification requirements. Nonconformance shall lead to immediate rejection of bid.

The certification shall state that the cab does meet or exceed the requirements below:

- 1) European Occupant Protection Standard ECE Regulation No. 29.
- 2) SAE J2422 Cab Roof Strength Evaluation - Quasi-Static Loading Heavy Trucks.

### **CAB MIRRORS, DRIVER ADJUSTABLE**

Section 14.3.5 of the NFPA 1901 Standards, 2009 edition, requires all primary rear view mirrors used by the driver to be adjustable from the driver's position.

### **CAB PAINT**

The finish paint and color as provided from the cab/chassis manufacturer shall be provided. Cab shall not be repainted.

(Note: Most departments do NOT find that the fleet paint finish from a commercial cab/chassis manufacturer is acceptable. The Body Builder will NOT be responsible for paint quality and finish issues.)

### **CAB INTERIOR COMPONENT PAINT COLOR, OEM SUPPLIED**

Powder coat shall be **matte** black.

### **HUB AND NUT COVERS**

If specified chassis supplied front and rear wheels hub caps and wheel nut covers shall be installed prior to delivery of completed unit.

### **MUDFLAPS**

There shall be 1/4" rubber mudflaps with logo provided and installed behind rear axle tires to prevent throwing road debris and lower road spray.

### **INSTALL CHASSIS SUPPLIED ON BOARD AIR COMPRESSOR**

An on board air compressor shall be shipped loose with the chassis and installed behind the drivers seat.

### **CHASSIS AIR TANK VALVES**

The cab/chassis air brake system tank drains shall be extended to Class 1 brass petcock valves with chrome plated zinc handle located on forward streetside lower body or as per tank locations. Each air tank and valve shall be inter-piped with black reinforced nylon tubing. Brass compression type fittings shall be used on the nylon tubing, meeting all DOT requirements.

Each handle shall be properly labeled to identify each tank.



## **ROAD EMERGENCY SAFETY KIT**

The DOT required reflective triangles, warning flares, and fire extinguisher shall be provided by cab and chassis supplier.

## **SIGTRONICS INTERCOM SYSTEM**

The following Sigtronics intercom system shall be provided and installed to improve the safety of firefighters and rescue professionals through enhanced communication and hearing protection. System shall have the following major components as minimum;

- Intercom Station, US-67D

## **MRIM-2 Mobile Radio Interface Module**

- Connects between your mobile radio, a single headset, and push-to-talk (PTT) switch – or use it to connect a cellular telephone to your intercom system.
- Allows two-way radio communication via the Sigtronics emergency headset.
- Used in high noise applications where radio communication is required, but vehicle intercom is not.
- All mounting hardware, jack box, switch box (PTT) and wire are included.
- Warranty: Two years parts and labor.

## **Switch Kit**

Sigtronics Patented Blue Box switch housing with 3PDT switch.

## **Sigtronics Emergency Radio Switcher SRS-6**

- The Emergency Radio Switcher allows AM / FM radio to be heard whenever intercom and / or mobile radio communications are not occurring.
- Our Radio Switcher is great for monitoring traffic and weather reports.
- AM / FM radio will not be heard over mobile radio, it will automatically be muted when communications occur.
- Warranty: Two years parts and labor.
- Radio interface for dual radio.

## **INTERCOM SYSTEM INSTALLATION**

The above listed intercom system headset jacks shall be installed in the cab locations as follows;

- Driver's – Intercom & radio PTT provided at driver position.
  - Position provided with under helmet headset model **SE-8 RVC**
  - Intercom headset jack shall be located overhead right shoulder.

- Push-to-Talk switch shall be located on center console/engine cover.
- Officer's
  - Intercom & radio PTT provided at officer position.
  - Position provided with under helmet headset model **SE-8 RVC**
  - Intercom headset jack shall be located overhead left shoulder.
  - Push-to-Talk switch shall be located on center console/engine cover.
  - Headset hook provided overhead left shoulder.

There shall be – (1) Intercom & radio PTT provision(s) provided in RC-1 rear compartment located on streetside.

- Position provided with under helmet headset model **SE-8 RVC**
- Headset shall be provided with radio PTT switch.
- Intercom headset jack shall be located on the streetside of the RC-1 Compartment
- **Headset hook provided on the RC-1 streetsdie wall.**

## **FRONT CAB INTERIOR COMPONENTS**

### **CHASSIS TIRE PRESSURE MONITOR SCREEN**

A chassis supplied tire pressure monitor screen shall be mounted in the chassis cab.

**Mounting location will be determined at mid inspection**



### **CHASSIS SUPPLIED VISTA**

There shall be a vista screen shipped loose from chassis manufacture for SVI to install on a swivel mount as shown in picture.

## **CREW CAB INTERIOR COMPONENTS**

### **REAR CAB INTERIOR BENCH SEAT**

The rear crew area of cab shall have a "U" shaped bench seat with minimum 20" seat cushion. The bench seat base shall be fabricated of 1/8" aluminum tread plate to form an under seat storage compartment.

The bench seat shall extend full width along the rear cab wall and along the street side and extending full width behind the engine tunnel to the curbside.

The seat shall be fabricated of 3/4" exterior grade plywood with 3" thick foam and matching black Durawear heavy duty fabric covering. The seat backrest shall be approximately 12" high x 2" thick and constructed the same as the seat.

There shall be hinged drop down access doors installed in the seat base. Two (2) Forward facing and Two (2) rear facing for access to the storage area below. There shall be no dividers between all the sections.

The access doors will be secured with paddle style latches.

Two (2) 18" OSS Acces Pro Led lights shall be installed in the forward facing underseat storage area and Two (2) 18" OSS Acces Pro Led lights shall be installed in the rear facing underseat storage area. The lights shall be activated by heavy duty door switches.

**The bench seats are designed for stationary use only and cannot be occupied while the vehicle is in motion.**

### **MULTI-THREAT CAB AIR FILTRATION UNIT**

Task Force Tips model # CC-300 CrewProtect air filtration system shall be provided. The unit shall purify the air by reducing particulates and Volatile Organic Compounds (VOCs). The Crew Protect shall also reduce aerosols carrying viruses and bacteria by over 99%.

The unit shall be mounted on the rear of the engine tunnel using the provided mounting brackets. The system shall run whenever the apparatus is operating. The unit shall have an air flow rate of 100 CFM (2832 cubic l/min) and operates at no more than 60.2 decibels, below the NFPA maximum of 90 decibels. The unit shall exchange the air every 3-1/2 minutes in an average apparatus cab of 350 cubic feet (9911 cubic liters).

The unit shall be in a protective steel case that is powder coated charcoal grey inside and out. The unit shall be 20" long, 12" wide and 4-1/2" tall (508 x 305 x 115 mm).

A single replacement filter element # CC-305 uses RFID technology to assure correct replacement filters are installed. Unit will not operate unless correct RFID filter is installed to provide protection for the crew. The current condition of the filter is tracked by three LED lights, green, amber, and red, on the prominent face of the unit.

The unit shall have a unique serial number and be covered by a three-year warranty.

**Shall activate with Ignition and V-MUX**

## **CAB MISCELLANEOUS EQUIPMENT**

The following items shall be provided in cab as follows;

### **120 VAC CAB OUTLETS**

- There shall be one (1) 120 VAC outlet(s) located **on officer side of engine tunnel rearward**.
  - The outlet receptacle(s) shall be 20 amp, straight-blade (NEMA 5-20R).
  - Outlet(s) shall be powered by both the on-board generator and shore power system through a relay system.

### **CAB COMMAND AREA - 120 VOLT A/C**

- **The chassis supplied RV air conditioner(s) shall be powered by gen/shore with auto relays.**

## **STREETSIDE FUEL FILL**

There shall be one (1) fuel fill door located in the streetside exterior wheel well panel, behind the rear axle. The fill door shall be fabricated from brushed stainless steel. There shall be a permanent label with the text "DIESEL FUEL ONLY" located adjacent to the fuel fill access.

## **CURBSIDE FUEL FILL**

There shall be one (1) fuel fill door located in the curbside exterior wheel well panel, behind the rear axle. The fill door shall be fabricated from brushed stainless steel. There shall be a permanent label with the text "DIESEL FUEL ONLY" located adjacent to the fuel fill access.

## **DEF FLUID FILL**

The DEF fluid fill shall be as supplied by commercial cab/chassis manufacturer.

## **BODY DESIGN**

The importance of public safety associated with emergency vehicles requires that the construction of this vehicle meet the following specifications. These specifications are written to establish the minimum level of quality and design. All Bidders shall be required to meet these minimum requirements.

It is the intent of these specifications to fully describe the requirements for a custom built emergency type vehicle. In order to extend the expected service life of this vehicle, the body module shall be removable from the chassis frame and be capable of being installed on a new chassis.

The sheet metal material requirements, including alloy and material thickness, throughout the specifications are considered to be a minimum. Since such materials are available to all Manufacturers, the material specifications shall be strictly adhered to.

The fabrication of the body shall be formed sheet metal. Formed components shall allow the Riverside County Fire Department to have the body repaired locally in the case where any object has struck the body and caused damage. The use of proprietary extrusions will prevent the Riverside County Fire Department from such repair and shall NOT be used. All fabricated body components to be cut by a laser or water-jet for superior cut edge quality.

Following construction of the subframe, which supports the apparatus body, the sheet metal portion of the body shall be built directly on the subframe. The joining of the subframe and body shall be of a welded integral construction.

The sheet metal fabrication of the body shall be performed using inert gas continuous feed welders only. The entire body shall be welded construction. The use of pop rivets in any portion of structural construction may allow premature failure of the body structure. Therefore, pop rivets shall NOT be used in the construction of the structural portions of the body. This includes side body sheets, inner panels of compartment doors, and any other structural portions of the body.

### **EXTERIOR ALUMINUM BODY**

The fabrication of the body shall be constructed from aluminum 3003H-14 alloy smooth plate. This shall include compartment front panel, vertical side sheets, side upper rollover panels, rear panels and compartment door frames.

The body compartment floors and exterior panels shall be constructed with not less than 3/16" (.187) aluminum 3003H-14 smooth plate. Interior compartment dividing walls shall be constructed with not less than 1/8" (.125) aluminum 3003H-14 smooth plate. Lighter gauge sheet metal will not be acceptable in these areas, No Exceptions.

The front and rear corners of body shall be formed as part of the front or rear body panels. This provides a stronger body corner and finished appearance. The use of extruded corners, or caps will not be acceptable, No Exceptions.

The door side frame openings shall be formed "C" channel design. An electrical wiring conduit raceway running the full length of exterior compartments shall be provided. This raceway shall contain all 12 volt wiring running to the rear of the apparatus, permitting easy accessibility to wiring.

Individual compartment modules, with dead air space voids between compartments, will not be an acceptable method of compartment construction.

The compartments shall be an integral part of the body construction. Compartment floors from front of body to ahead of rear axle, also from rear axle to rear of body shall be single one-piece sections. Compartment floors shall be preformed, then positioned in body and welded into final position.

Compartment floors shall have a "sweep-out" design with door opening threshold positioned lower than compartment floor, permitting easy cleaning of compartments. Angles, lips, or door moldings are not acceptable in the base of compartment door opening. One-way rubber drain valves shall be provided in compartment floors so that a water hose may be used to flush-out compartment area.

All exterior seams in sheet metal below frame, and around the rear wheel well area shall be welded and caulked to resist moisture from entering the compartments. All other interior seams and corners shall be sealed with silicone based caulk prior to painting.

Only stainless steel bolts, nuts, and sheet metal screws shall be used in mounting exterior trim, hardware and equipment.

### **DRIP RAILS**

The body shall have drip rails over the side full height compartments. The drip rails shall be formed into the upper body panels providing a ridged lower panel and a flat upper body panel surface. The use of mechanically fastened, taped or glued on drip rails will not be acceptable, No Exceptions.

## **ROOF CONSTRUCTION**

The roof structure shall be integral with the body sheet metal construction and shall be an all welded assembly. The body roof structure shall be overlaid with not less than 3/16" aluminum 3003H-14 alloy tread plate and welded to roof structure and body sheet metal. All seams in roof material shall be fully and continuously welded to resist entry of moisture.

There shall be a total of four (4) 2" x 2" x 1/4" 6061-T6 alloy aluminum "C" channels running the length of body, two (2) on each outboard side. These "C" channels shall be used for roof support and in addition shall be used for mounting of any specified reels. This open "C" channel design along with special reel mounting clips allows for a universal location of any specified reels within each compartment.

In between the two (2) center "C" channels running the length of body shall be 2" x 2" x 1/4" 6061-T6 alloy aluminum tubing running in between and welded in place on approximate 16" centers to support roof and/or walkway structure if specified.

A 2" formed radius shall be provided along the body sides and utilized as a wiring trough. The use of aluminum extrusions in this area shall not be acceptable, .

## **BODY SUBFRAME**

The chassis frame rails shall be fitted with 1/4" custom extruded UHMW polyethylene rail cap to isolate the body frame members from direct contact with chassis frame rails.

The body subframe shall be constructed from 6061T6 aluminum alloy tubing. Subframe shall consist of two (2) 2" x 6" x 1/4" aluminum tubes, the same width as the chassis frame rails, NO EXCEPTION. Welded to this tubing shall be cross members of 2" x 6" x 1/4" aluminum. These cross members shall extend the full width of the body to support the compartments. Cross members shall be located at front and rear of the body, below compartment divider walls, and in front and rear of wheel well opening. Additional aluminum cross members shall be located on 16" centers, or as necessary to support walkway or heavy equipment.

To form the frame, the tubing shall be beveled and welded at each joint using 5356 aluminum alloy welding wire.

## **BODY MOUNTING**

The body subframe shall be fastened to the chassis frame with six (6) spring loaded body mounts. Each mount shall be configured using a two-piece encapsulated slide bracket. The two (2) brackets shall be fabricated of heavy duty 1/4" thick steel and shall have a powder coat finish to resist any corrosion. Each mounting assembly shall utilize two (2) 3/4" diameter x 6" long grade 8 bolts and two (2) heavy duty springs. The assembly design shall allow the body and subframe to act as one (1) component, separate from the chassis. As the chassis frame twists under driving conditions, the spring mounting system shall eliminate any stress from being transferred into the body. The spring loaded body mounts shall also prevent frame side rail or body damage caused by unevenly distributed stress and strains due to load and chassis movement.

Body mountings that do not allow relief from chassis movement will not be acceptable.

## **10" REAR STEP BUMPER**

The full width rear bumper shall be constructed from 2" x 2" x 1/4" aluminum tubing frame and covered with 3/16" NFPA compliant aluminum tread plate. The bumper shall extend from the rear vertical body panel 10" and provide a rear step with a minimum of 1/2" space at body for water drainage.



### **REAR TOW EYES**

There shall be two (2) heavy duty rear mounted tow eyes securely attached to the body subframe, below body. The tow eyes shall be fabricated from 3/4" thick steel plate with a 3" diameter opening. Tow eyes shall have a black powder coat finish.

### **GROUND LIGHTS**

There shall be two (2) OnScene 8" Access white LED lights installed below bumper capable of providing illumination at a minimum level of 2 fc (20 lx) on ground areas within 30 in. (800 mm) of the edge of the vehicle in areas designed for personnel to climb onto or descend from the vehicle to the ground level.

Lighting shall be switchable but activated automatically when the vehicle park brake is set.

### **WHEEL WELL EXTERIOR PANEL**

The exterior panel of the body wheel well enclosure shall be constructed from 3/16" smooth aluminum panels.

### **STAINLESS STEEL BODY FENDERETTES**

The body wheel well openings shall be provided with round radius, polished stainless steel fenderettes. The fenderettes shall be bolted and easily replaceable if damaged. The fenderettes shall be installed using a rubber gasket to reduce buildup of moisture and/or debris.

### **WHEEL WELL LINERS**

The wheel wells shall be provided with an easily removable polymer, circular inner fender liner. The inner liner shall be bolted to the wheel well with stainless steel bolts and spaced away from the wheel well so the liner will not accumulate dirt or water.

### **GARDEN HOSE OUTLET COMPARTMENTS**

Two garden hose/misting system compartments shall be provided, one (1) each side of the body in rear wheel well area. Each compartment shall have a brushed SST door assembly with a positive catch latch, (to match the fuel fill doors). Each compartment shall be set up to hold the garden hose outlet and misting system outlet. The door shall activate the "Hazard Warning Light" in the cab when not in the closed position.



**NOTE: Match layout to previous unit for Riverside County #996**

## **BODY PAINT SPECIFICATIONS**

### **BODY PAINT PREPARATION**

After the body and components have been fabricated they shall be disassembled so when vehicle is complete there shall be finish paint beneath the removable components. The body shall be removed from chassis during the paint process to insure proper paint coverage. The body and components shall be metal finished as follows to provide a superior substrate for painting.

The exterior (and interior, if painted) body shall undergo a thorough cleaning process starting with a biodegradable phosphoric acid solution to begin the etching process followed by a complete clear water rinse. The next step shall consist of a chemical conversion coating applied to seal the metal substrate and become part of the metal surface for greater film adhesion.

All bright metal fittings, if unavailable in stainless steel or polished aluminum, shall be chrome plated. Iron fittings shall be copper under plated prior to chrome plating.

### **PAINT PROCESS**

The paint process shall follow the strict standards set forth by PPG Industries guidelines. Painters applying PPG products will be PPG Certified Commercial Technicians, and re-certified every two (2) years. The body shall go through the following paint process;

- 1) Clean bare metal with a wax and grease remover using low lint rags.
- 2) Inspect, straighten, and hammer high points, grind all seams, sharp edges, and welds. DA sand entire paintable surfaces using 24-180 grit dry paper. Plastic fill all low spots and DA sand fill areas using 36-180 grit dry paper. Apply pinhole filler and DA sand areas using 80-180 grit dry paper.
- 3) Re-clean bare metal using a wax and grease remover and low lint rags.
- 4) Within 24 hours, a PPG Delfleet® epoxy color primer with proper hardener for corrosion resistance using a pressure pot spray gun and applying 2-5 full wet coats or 1.5-8.0 dry mils max. achieving full hiding and allow to air dry 60 minutes @ 70°F or bake for 45 minutes @ 140°F degree.
- 5) Inspect, putty fill, and dry guild coat entire body surface and DA sand using 180-400 grit dry paper.
- 6) Re-clean bare metal using a wax and grease remover using low lint rags.
- 7) A PPG Delfleet® primer sealer with proper hardener and thinner shall be sprayed using a pressure pot spray gun and applying 1 full wet coat or 1.0-2.0 dry mils achieving full hiding and allow to flash off in spray booth for minimum of 60 minutes @ 70°F.
- 8) A PPG Delfleet® FBCH basecoat (color) with proper hardener and dry additive shall then be sprayed using a pressure pot set @ 45-60 PSI and achieving full hiding or 1.5-2.0 wet mils and allow to flash off in spray booth 45-60 minutes before applying clearcoat.
- 9) A PPG Delfleet® clearcoat with proper hardener and thinner shall be sprayed using a pressure pot spray gun and applying 2-3 full wet coats or 5.0 wet mils for a uniform gloss and allow to flash off in spray booth 10 minutes and bake for 120-140 minutes @ 125°F (surface temp.).
- 10) After cooling, DA sand heavy orange peel or runs using 1000 grit dry sand paper and final DA sand using 1500-2000 grit dry sand paper. Wipe off all surfaces to remove dust and debris. Buff unit as needed using 3M rubbing compound and a white wool pad and inspect until all sand scratches are removed.
- 11) Polish as needed using 3M Perfect-It-Polish and a black foam pad, repeat as necessary and inspect until all sand scratches are removed.

## **PAINT - ENVIRONMENTAL IMPACT**

The contractor shall meet or exceed their current State regulations concerning paint operations pollution control and shall include measures to protect the atmosphere, water and soil. PPG Delfleet® Evolution paint shall be free of all heavy metal (lead & chromate) components. Paint emissions from sanding and painting shall be filtered and collected. All paint wastes shall be disposed of in an environmentally safe manner. Solvents used in cleanup operations shall be collected, sent off-site for distillation and returned for reuse.

## **FASTENERS**

Prior to the assembly and reinstallation of exterior components; i.e. warning and DOT lights, handrails, steps, door hardware, and miscellaneous items, a Mylar isolation tape, or gasket shall be used to prevent damage to the finish painted surface. These components shall be fastened to body using either a plastic insert into body metal with stainless steel screws or zinc coated nut-surts into body surface using stainless steel bolts to resist corrosion from dissimilar metals.

## **ELECTROLYSIS CORROSION CONTROL**

The vehicle shall be assembled using ECK brand or similar corrosion control compound on all high corrosion potential areas.

ECK protects aluminum and stainless steel against electrolytic reaction, isolates dissimilar metals and gives bedding protection for hardware and fasteners. ECK contains anti-seizing lubricant for threads. ECK is dielectric and perfect for use with electrical connectors.

## **PAINT FINISH - SINGLE COLOR**

The body shall be painted with a single color of PPG Delfleet® Evolution per Riverside County Fire Department approved paint spray out provided.

- Paint Color: Match cab/chassis supplied paint color.  
**FBCH-992088 RED**

## **BODY UNDERCOATING**

The entire underside of body shall be sprayed with black automotive undercoating. Undercoating shall cover all areas underside of body and wheel well area to help resist corrosion under the vehicle.

## **COMPARTMENT INTERIOR FINISH**

The interior of all exterior body compartments shall be a "Maintenance Free" smooth unpainted finish. All body seams shall be finished with a caulk sealant for both appearance and moisture protection.

## **REFLECTIVE STRIPE REQUIREMENTS**

### **Material**

All retroreflective materials shall conform to the requirements of ASTM D4956, *Standard Specification for Retroreflective Sheeting for Traffic Control*, Section 6.1.1 for Type I Sheeting.

All retroreflective materials used that are colors not listed in ASTM D4956, Section 6.1.1, shall have a minimum coefficient of retro-reflection of 10 with observation angle of 0.2 degrees and entrance angle of -4 degrees.

Any printed or processed retroreflective film construction used shall conform to the standards required of an integral colored film as specified in ASTM D4956, Section 6.1.1.

### **Minimum Requirements**

A retroreflective stripe(s) shall be affixed to at least 50 percent of the cab and body length on each side, excluding the pump panel areas, and at least 25 percent of the width of the front of the vehicle, not including mirrors or other protrusions.

The stripe or combination of stripes shall be a minimum of 4 in. (100 mm) in total width.

The 4 in. (100 mm) wide stripe or combination of stripes shall be permitted to be interrupted by objects (i.e., receptacles, cracks between slats in roll up doors) provided the full stripe is seen as conspicuous when approaching the apparatus.

A graphic design shall be permitted to replace all or part of the required striping material if the design or combination thereof covers at least the same perimeter length(s).

## **GRAPHICS PROOF REFERENCE SIGNED APPROVAL ALSO**

A color graphics proof of the reflective striping layout shall be provided for approval by Riverside County Fire Department prior to installation. The graphics proof shall be submitted to Riverside County Fire Department on 8.5" x 11" sheets with front, sides, rear and plan views, each on one (1) sheet. In addition if there is any special art work an additional sheet shall be provided showing all details. **Note:** The graphics color proof may not reflect the correct paint break lines on the chassis and body please refer to the paint section of your specifications for correct paint break lines.

### **REFLECTIVE STRIPE - CAB SIDE**

The reflective stripe material shall be 6" wide, 3M Scotchlite 680 series graphic film.

- This reflective stripe shall be white in color.

### **REFLECTIVE STRIPE - CAB FRONT**

The reflective stripe material shall be 6" wide, 3M Scotchlite 680 series graphic film.

- This reflective stripe shall be white in color.

### **CHEVRON STRIPE - CAB BUMPER**

A reflective stripe shall be affixed to the front of cab. The stripe or combination of stripes shall be a minimum of 4 in. (100 mm) in total width.

The approximate 10" wide Chevron retroreflective stripe shall be affixed to at least 25 percent of the width of the front of the apparatus with retroreflective striping in a chevron pattern sloping downward and away from the centerline of the vehicle at an angle of 45 degrees. Each stripe shall be 6" width. Chevron panels shall have a 3M UV over laminate to protect from UV rays, scene damage, and everyday use. Chevron panels shall have a minimum 10 year warranty for material failure, and colorfastness.

- The stripe material shall be 3M Scotchlite 680 series graphic film.

All retroreflective materials required shall conform to the requirements of ASTM D 4956, *Standard Specification for Retroreflective Sheeting for Traffic Control*, Section 6.1.1 for Type I Sheeting.

- This reflective stripe shall be white in color.

### **REFLECTIVE STRIPE - CAB DOOR INTERIOR**

Any door of the apparatus designed to allow persons to enter or exit the apparatus shall have at least 96 in.2 (62,000 mm2) of retroreflective material affixed to the inside of the door.

The inside of each cab and crew doors shall have 4" Chevron style diamond grade reflective striping. The colors shall be red and fluorescent yellow-green.

### **REFLECTIVE STRIPE - BODY SIDES**

The reflective stripe material shall be 6" wide, 3M Scotchlite 680 series graphic film.

- This reflective stripe shall be white in color.

The stripe shall extend straight from front of cab, then ahead of the rear wheels, it shall form an "S" shape and extend straight back to the rear of the body. The "S" portion of the stripe shall have a black shading in the corners.

### **CHEVRON REFLECTIVE STRIPE - REAR CENTER/SIDE PANELS**

At least 50 percent of the rear-facing vertical surfaces, visible from the rear of the apparatus, excluding any pump panel areas not covered by a door, shall be equipped with retroreflective striping in a chevron pattern sloping downward and away from the centerline of the vehicle at an angle of 45 degrees. Each stripe shall be 6" width.

The rear side panels and center of the body shall have a chevron style reflective stripe, extending from bumper height up to side compartment drip rail height. Chevron panels shall have a 3M UV over laminate to protect from UV rays, scene damage, and everyday use.

The stripe material shall be 3M Scotchlite 680 series graphic film.

This reflective chevron stripe shall alternate red and yellow in color.

## **LETTERING**

### **GRAPHICS PROOF**

A color graphics proof of the lettering layout shall be provided for approval by Riverside County Fire Department prior to installation. The graphics proof shall be submitted to Riverside County Fire Department on 8.5" x 11" sheets with front, sides, rear and plan views, each on one (1) sheet. In addition if there is any special art work an additional sheet shall be provided showing all details.

The following lettering shall be provided and installed on the completed unit as follows;

### **SIDE CAB DOOR LETTERING**

### **UPPER BODY SIDE LETTERING**

### **REAR BODY LETTERING**

### **FRONT OF CAB LETTERING**

### **EXTERIOR COMPARTMENT DOORS**

## **ROLL-UP DOOR CONSTRUCTION - AMDOR**

The apparatus shall be equipped with Amdor brand exterior roll-up compartment doors. Amdor roll-up doors shall be complete with the following features; **Doors will have Anodized tracks.**

- 1" aluminum double wall slats with continuous ball & socket hinge joint and recessed dual durometer slat seal
- Double wall reinforced bottom panel with stainless steel lift bar latching system
- Bottom panel flange with cut-outs for ease of access with gloved hands
- Reusable slat shoes with positive snap-in securement
- Smooth interior door curtain to prevent equipment hang-ups
- One-piece aluminum door track / side frame, top gutter with non-marring seal
- Non-marring recessed side seals with UV stabilizers to prevent warping
- Dual leg bottom seal, with all wear component material to be Type 6 Nylon
- The door shall be warranted for a period of 36 months from the date of delivery. AMDOR Inc. liability covers the replacement or repair of any component that fails due to defects in material and / or workmanship during the coverage period.

Each shutter door shall decrease the compartment door frame opening approximately 2.00" in width and approximately 5.50" in height for the bottom section of door assembly.

The specified retroreflective stripe material shall be applied on the roll-up compartment doors. The stripe shall be precision machine cut for each door slat of the roll-up doors. Under no circumstance will the stripe material be cut on roll-up door surface.

## **BODY HEIGHT MEASUREMENTS**

The vertical body dimensions shall be as follows:

### **AHEAD OF REAR AXLE**

	<u>Description</u>	<u>Dimension</u>
A	Bottom of Subframe to Top of Body	84.0"
B	Bottom of Subframe to Bottom of Body	22.5"
C	Vertical Door Opening	
	-with roll-up door	67.5"
	-with hinged door	71.0"

### **ABOVE REAR AXLE**

	<u>Description</u>	<u>Dimension</u>
D	Vertical Door Opening - Above Rear Wheel	
	-with roll-up door	34.0"
	-with hinged door	37.5"

### **BEHIND REAR AXLE**

	<u>Description</u>	<u>Dimension</u>
E	Bottom of Subframe to Bottom of Body	20.0"
F	Vertical Door Opening	
	-with roll-up door	62.0"
	-with hinged door	65.5"

### **GENERAL**

<u>Description</u>	<u>Dimension</u>
--------------------	------------------

G	Bottom of Drip Rail to Top of Body	33.5"
---	------------------------------------	-------

(Dimensions are approximate and subject to change during the actual design process.)

**BODY WIDTH DIMENSIONS**

The body shall be 100.0" wide, and 102.0" wide at drip rails. Interior compartment depth dimensions shall be approximately:

<u>Area Description</u>	<u>Dimension</u>
Transverse above subframe	95.0"
Compartment depth below subframe	24.5"



## **STREETSIDE COMPARTMENT - FRONT (S1)**

The interior useable compartment width shall be approximately 56.5" wide.

### **SIDE ENTRY DOOR**

Access shall be provided to the interior through a single side entry door with a clear door opening width of approximately 28.5".

Construction of the side entry door shall be with 1/8" aluminum exterior smooth plate and painted exterior body color choice. The interior door panel shall be constructed from 1/8" aluminum treadplate.

The door shall be hung on full height 14 gauge stainless steel hinge, with a 1/4" stainless steel pin. The hinge shall be bolted to the door and body with stainless steel machine screws at offset 5" centers. A polyester barrier film gasket shall be placed between the stainless steel hinge and door.

Full width padded foam cushion head bumper shall be provided above door opening. The head bumper shall be covered with matching interior vinyl and bolted to interior of door way.

The door latch mechanism shall include a stainless steel paddle type handle on interior. A polyester barrier film gasket shall be placed between the stainless steel handles and the aluminum door panels. The door latch shall be a double catch two-point safety slam latch recessed inside the double panel door with strike plate mounted top and bottom of door frame complying with FMVSS requirements.

- The hinged door(s) shall have a stainless steel 6" offset bent D-ring locking handle. A gasket shall be placed between handle and door. Door latches shall be a two-point rotary slam, double-catch latch, recessed inside the double panel door with striker plate.

### **WINDOW(S)**

There shall be one (1) 18" wide x 22" high, double-paned insulated, non-sliding window(s) installed in the entrance door. Each window shall have tinted automotive type safety glass mounted in an extruded aluminum frame. The frame shall have a black anodized finish.

**The window shall be opaque**

- One (1) OnScene 8" Access white LED ground light(s) shall be provided below the body. Light(s) shall be switchable but activated automatically when the park brake is set.

### **ENTRY HANDRAILS**

There shall be two (2) handrails provided at entry door; one (1) Hansen International 24" x 1-1/8" vertical handrail on exterior of body on door handle side, and one (1) Hansen International 30" x 1-1/8" on inside of door. The interior handrail shall be angled for optimum use when entering or exiting the interior body area. Handrails shall be NFPA compliant formed from anodized aluminum with knurled anti-slip finish.

Each handrail shall be back-lit with a Safetylite, 12 VDC white LED light tube. Lights shall be activated with headlight and park brake set circuits.

A safety sign FAMA23, which warns of the proper climbing method, shall be visible to personnel entering the cab and at each designated climbing location on the body.

A safety sign FAMA24, which warns personnel not to ride on the vehicle, shall be located at the rear step areas and at any cross walkways.

### **ELECTRIC STEP**

There shall be one (1) Kwikkee 39 Series 12 VDC, electric step(s) that automatically extends when you open entry door(s) and retracts when you close entry door(s). The power step will automatically stop if it strikes an obstacle. The Kwikkee electric step components uses weatherproof wiring and connectors to prevent shorts and corrosion in the system.

The distance from the ground to the first step shall be no more than 24" per in accordance with NFPA 1901 guideline. The top surface of each step shall be covered with an NFPA 1901 nonskid compliant aluminum tread plate.

### **LAVATORY COMPARTMENT**

This vehicle shall be provided with an enclosed lavatory compartment with full height hinged entry door. The compartment walls and ceiling shall be covered with gray pebble grain FRP panels. A Fantastic model 6000RBTA, 12 VDC, 3-speed ventilation fan(s) shall be provided for air circulation. An OnScene LED 10" x 10" 12 VDC white interior light shall be provided on ceiling with a switch at the door. A toilet paper roll dispenser shall be provided in the compartment.

**Floor will be treadplate for easy washout.**

### **INTERIOR WATER SYSTEM**

There shall be one (1) **100** gallon plastic fresh water holding tank(s) located below the apparatus body. A fresh water fill shall be provided at the exterior apparatus body with a household hose type connection. A 12 volt self priming, flow controlled water pump (minimum of 3 GPM) with built-in check valve shall be provided and plumbed to water system.

An Integrity RV tank level monitor system (or equal) shall be provided and installed on completed unit. The monitor shall be located in practical location for monitoring and include a 2 x16 LCD backlit screen to monitor the on-board fresh water tank(s) level, and the black water holding tank(s) level.

There shall be one (1) **120 USG** gallon plastic holding tank(s) located below the apparatus body. There shall be an RV type waste water drain system installed using flexible tube. There shall be a valve located below the apparatus body to drain the retention tank.

A Thetford SaniCon (or equal) RV tank drain system shall be provided and installed. The SaniCon tank drainage system is the cleanest, most sanitary way to empty a holding tank. The heavy-duty transfer pump macerates waste, sending it up to 20' up hill. Permanent connections shall be provided to save handling and setup time, and keep you clean. The long lasting 1" discharge hose stretches to 21' yet collapses to 7' long to save storage space. The easy to use nozzle adapts to fit a variety of dump station, no need for adapters. System include a fuse and switch.

There shall be one (1) permanently mounted RV Quickee Flush waste tank rinser provided. The tank rinser shall include a permanently installed built-in back flow preventer and a standard garden hose type hook-up.

No water heater system shall be provided with specified sink system.

## **WATER/WASTEWATER ACCESS DOOR**

There shall be one (1) vertically hinged door with a D-ring handle provided on the lower front of the streetside body. The door shall be designed to provide access to the fresh water tank fill, waste water tank drain, and any other water system access points. Additionally, a storage area shall be provided for waste removal hose(s) and fill hose(s).

There shall be one (1) three (3) position fill valve provided. The valve shall have positions for filling both fresh water tanks simultaneously or operation from external water supply.

## **LAVATORY TOLIET**

There shall be one (1) RV style, permanent toilet(s) installed in the lavatory compartment. The toilet shall be a stainless steel base model. The toilet shall be plumbed to the water system, providing fresh water for the flush cycle and a gray water tank for disposal.

## **LAVATORY SINK**

The lavatory sink design shall be small and compact. Countertop and sink enclosure shall be constructed of **brushed stainless**.

A stainless steel sink shall be provided and recessed into countertop. The sink shall be provided with chrome plated faucet with individual control valves for cold or hot (if specified) water.

No water heater system shall be provided with specified sink system.

## **AIR CONDITIONER - HEATER**

One (1) Dometic Penguin II low profile, 120 VAC, 60 cycle, single phase air conditioner(s) shall be provided and installed on roof of vehicle. The unit shall be a roof top contemporary contoured integral evaporator/condenser type with built-in heating elements.

Each unit shall be rated at minimum of 13,500 BTU cooling capacity with a heating element rated at 5,600 BTU. A three-speed fan shall supply a maximum/minimum of 320/250 cfm air flow capacity. Air conditioner(s) shall be controlled by a wall mounted Comfort Control II LCD thermostat.

The roof mounted air conditioner shall be approximately 9.5" high x 29" wide x 40" long and weigh approximately 99 lbs.

- The above rooftop Air Conditioning units shall be powered by both the generator and shore power
- The thermostat(s) for the above rooftop Air Conditioning units shall be located above the interior light switch panel.

## **EXHAUST FAN**

One (1) Fantastic model 6000RBTA, 12 VDC, 3-speed ventilation fan(s) shall be provided for air circulation. Each fan shall be wired to a wall switch located near fan location.

### **Technical Information:**

- Durable, proven longevity
- Quiet, 12 – volt ceiling fan with 3-speeds
- Polycarbonate dome/Lifetime guarantee
- Removable screen for easy cleaning
- Reversible fan blade motor (in or out)
- Low AMP draw insures full-time use

Performance:	SCFM	AMPS	Decibels
High	920	3.00	40
Medium	653	2.29	39
Low	478	1.86	39

### **Specifications:**

- Rooftop weight: 11lbs.
  - Dimensions: 16 1/2 x 16 1/2 x 4 1/2 (Fits Most Standard 14"x14" Openings)
  - CSA / UL Certified
- Specified roof vent shall be provided with a Maxxair model 00-933069 black vent cover.

There shall be two (2) Whelen surface mount ION Series LED light(s) with wide angle optic provided, one (1) each side. The light head shall include an integral flasher with programmable flash patterns.

Each light shall have:

- Red LEDs
- Clear Lens
- Chrome Flange

The lights shall be controlled at **Lavatory door switch**.

- The 12 volt electrical distribution panel shall be located in the front lower compartment.

## **STREETSIDE COMPARTMENT - AHEAD OF REAR WHEELS (S2)**

The interior useable compartment width shall be approximately 41.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 35.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

## **COMPARTMENT LAYOUT**

- There shall be vertically mounted aluminum Shelf-Trac welded to compartment walls for specified component installation. Shelf-Trac extrusion shall have side extruded channels for use in mounting or securing special ancillary items, without need for drilling into body.
- There shall be three (3) adjustable shelf/shelves approximately 70" deep. Each shelf shall be fabricated from 3/16" 3003 aluminum sheet with a 2" vertical flange along the front and rear edges.
  - Any equipment mounting on adjustable shelf shall be provided by Riverside County Fire Department after delivery.
  - The above component(s) shall have a smooth un-painted finish.
  - 3M™ Diamond Grade™ Conspicuity striping shall be provided on the front face of the shelf(s).
- This reflective stripe shall be red/white in color.

- One (1) Bauer complete portable SCBA filling station(s) shall be provided with the delivered apparatus. Fill station shall be used in remote locations in conjunction with an (optional) portable fragmentation shield.

The high pressure suitcase shall be constructed of injection molded ABS plastic, safety yellow in color and shall be equipped with a full o-ring seal to insure its protection from the environment.

It shall not exceed 21-1/2" in length by 14" in depth and 9" in height and must not exceed a total weight of 23 lbs.

The components inside shall consist of the following:

- Inlet control valve
- Inlet pressure gauge
- High pressure bleed valve
- Adjustable regulator from 1,000 to 6,000 psi.
- Regulated pressure gauge
- Relief valve protecting secondary side of regulator
- Two (2) flexible 5' filling whips with bottle filling attachments, bleed valves and safety fill adapters

All of the above equipment shall be mounted on a (.062) zinc plate with a water resistant brushed finish. The labeling and flow diagram shall be engraved into the mounting plate and shall be color coded for ease of operation. The internal plumbing shall be done with (.049) seamless stainless steel tubing and stainless fittings. The entire system shall be designed with a minimum 4 to 1 safety factor. The mounting plate shall be made in two (2) pieces allowing the right side plate to be hinged creating a storage compartment for the two (2) filling whips with attachments.

- The floor of the compartment above the frame rails shall be extended to the interior edge of the door. The floor shall have a 2" vertical lip and a 1" return to increase strength.
- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.
- There shall be one (1) 120 VAC **4-gang** outlet(s) located in compartment.
  - The outlet receptacle(s) shall be 20 amp, straight-blade (NEMA 5-20R).
  - Outlet(s) shall be powered by both the on-board generator and shore power system through a relay system.
  - The outlet shall be located on forward wall, lower left area.
- There shall be one (1) underbody slide-out step. Step surface shall be constructed from 9" deep DiamondBack non-slip vented aluminum stair treads mounted to underbody using Delron plastic slides for corrosion resistance. Step slide shall be securely held in both out and stored position, utilizing a heavy duty pneumatic cylinder designed to have an over center location which will assist the step in both extension and retraction. Each step shall be designed to hold 500 lbs.
- One (1) OnScene 9" Night Axe white LED ground light(s) shall be provided below the body. Light(s) shall be switchable but activated automatically when the park brake is set.
- Two (2) 3-1/2" x 3-1/2" black plastic louvered vents shall be provided in the lower compartment.

### **STREETSIDE COMPARTMENT - ABOVE REAR WHEELS (S3)**

The interior useable compartment width shall be approximately 64.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 58.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

### **COMPARTMENT LAYOUT**

- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.
- A Bauer model K-22.42-30-E3 air compressor with a recharging rate of 35.9 SCFM @ 6,000 PSI shall be provided, . Compressor skid shall include 30 HP, 3-phase soft start electric motor, P10 Securus purification system, electronic CO monitor and calibration kit, and fill station inter-connecting harness. Compressor module shall be approximately 58" L x 56" W x 54" H and weigh 1,950 pounds.

High pressure air hose and couplings are to have a pressure rating equal to or greater than the highest pressure expected to be encountered, with a safety factor of 4 to 1.

- Air storage shall consist of four (4) ASME 491 SCF @ 6,000 PSI, (does not require hydrostatic testing) shall be provided on completed vehicle complete with gauges and valves. Each cylinder shall measure 9.6" diameter x 55" long, and weigh 400 lbs.

The manufacturer's test date (month and year) on each air tank shall be current within 12 months of the apparatus delivery date.

Air tanks shall be marked with a label that reads;

“High Pressure 6,000 PSI Breathing Air” or “High Pressure 41,368 kPa Breathing Air.”

High pressure air hose and couplings are to have a pressure rating equal to or greater than the highest pressure expected to be encountered, with a safety factor of 4 to 1.

- There will be a welded reinforcement above the body frame to carry specified DOT or ASME cylinders. The mounting of the cylinders will be with adjustable track and powder coated steel band straps to securely hold all cylinders in place.
- An Appleton inlet and base shall be provided in compartment near compressor. The compressor shall have a 2/00 AWG SO cord with a matching Appleton plug for operating compressor from the on-board generator system. Another matching Appleton plug shall be provided with completed vehicle for operating the compressor from an in-house electrical system. All required building wiring shall be responsibility of Riverside County Fire Department.
- The Bauer compressor shall be free from defects in material and workmanship for a period of two (2) years. The foregoing warranty period shall be extended to five (5) years from the date of shipment from Bauer for Customers that are Municipal Fire Departments with respect to the compressor block (breathing air application), provided that such extended warranty period shall only apply to product parts with proof of proper maintenance being completed in accordance with published Bauer factory recommendations. To be eligible for this limited warranty to cover Customer's product, Customer must return a properly completed start-up/warranty registration form to Bauer within ninety (90) days from the date of start-up.
- One (1) day of training and instruction shall be provided by compressor manufacturer per NFPA 24.2.13 at Riverside County Fire Department location on proper use of air compressor, purification system, filling of SCBA, and air reel operations, if specified.
- The NFPA required air quality test shall be completed by manufacturer prior to delivery. Complete results of test shall be provided to Riverside County Fire Department upon delivery.



## **STREETSIDE COMPARTMENT - REAR (S4)**

The interior useable compartment width shall be approximately 64.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 58.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

## **COMPARTMENT LAYOUT**

- There shall be vertically mounted aluminum Shelf-Trac welded to compartment walls for specified component installation. Shelf-Trac extrusion shall have side extruded channels for use in mounting or securing special ancillary items, without need for drilling into body.
- There shall be one (1) Austin Front Drawer Release (FDR) 400 lbs. slide-out tray(s) approximately 30" deep and as wide as the compartment layout or door opening permits. **Tray will have a work surface.**  
Each tray shall be vertically adjustable. The FDR on front of tray will deduct 1.5" from specified depth. The tray top shall be fabricated from 3/16" 3003 aluminum sheet with a 3" vertical lip and welded corners to form a box type tray surface. The sliding tracks shall extend 100% of the slide length.
  - Any equipment mounting on slide tray shall be provided by Riverside County Fire Department after delivery.
  - The above component(s) shall have a smooth un-painted finish.
  - 3M™ Diamond Grade™ 2" wide conspicuity striping shall be provided on the front face of the tray.
- This reflective stripe shall be red/white in color.

- There shall be one (1) SCBA cylinder storage module for 7-5/8" OD (maximum) SCBA bottles. The maximum length of the SCBA cylinder shall be 24.75". The module shall have an exterior shell fabricated from 1/8" (.125) 3003H-14 aluminum alloy sheet. The module shall have a 2" slope, front to back to prevent cylinders from sliding out. The SCBA cylinder storage tubing shall be fabricated from PVC pipe to resist damage or abrasion to cylinders. In addition there shall be rubber pad provided in the base of each storage tube for bottle protection and to resist slipping.
  - The SCBA cylinder module shall be capable of storing sixteen (16) SCBA cylinders up to 7-5/8" diameter.
- There shall be two (2) Zico ULLH Load & Lock walkaway type SCBA air pack bracket(s) with "V" type clip and strap assembly to hold SCBA in place.
- The floor of the compartment above the frame rails shall cover the area directly above the frame rails ONLY (non-extended floor).
- One (1) Hannay ECR1618-17-18 electric cable reel(s) capable of storing 200' of 10/3 electric cable. Reel(s) shall be designed to hold 110% of the capacity of cord length, with fully enclosed 45 amp, three (3) conductor collector rings. Reel(s) shall be mounted to channel structure that allows for side-to-side adjustment of reel position.
  - Power rewind control(s) shall be in a position where the operator can observe the rewinding operation and not be more than 72 in. (1830 mm) above the operator's standing position, and shall be marked with a label indicating its function and shall be guarded to prevent accidental operation.
  - A label shall be provided in a visible location adjacent to reel with following information: Current rating, Current type, Phase, Voltage, and Total cord length.
    - The cable reel shall equipped with 200' of 10/3 SEOW black cable, a molded plastic ball clamp, and a single heavy duty L5-30 twist-lock female plug at the end.
- One (1) Akron model EJBX series, cast aluminum electrical power distribution box with gray powder coat painted finish shall be provided. The power distribution box shall meet all requirements described in NFPA 1901. The power distribution box shall include the following outlets mounted on a backlit face plate;
  - A 12" pigtail that terminates in an L5-30 configuration to match the cable on the cord reel. The outlet configuration shall include:
    - One (1) 120 VAC, 5-20 duplex straight-blade receptacle
    - One (1) 120 VAC, 5-20 duplex straight-blade receptacle
    - One (1) 120 VAC, L5-20 single twist lock receptacle.
    - One (1) 120 VAC, L5-20 single twist lock receptacle.
- One (1) Akron Brass model EJB-VMT aluminum treadplate vertical mounting bracket for specified power distribution box shall be provided and mounted in compartment per Riverside County Fire Department.
- The fairlead roller shall be mounted directly to the reel.
- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.

- There shall be one (1) 120 VAC **4-gang** outlet(s) located in compartment.
  - The outlet receptacle(s) shall be 20 amp, straight-blade (NEMA 5-20R).
  - Outlet(s) shall be powered by both the on-board generator and shore power system through a relay system.
  - The outlet shall be located on forward wall, lower left area.

### **TOOL MOUNTING**

**PAC 1003 HD as specified in the equipment section shall be installed on the aft wall for customer supplied 6' Rubbish hook and 6' NY Roof hook**

- There shall be one (1) underbody slide-out step. Step surface shall be constructed from 9" deep DiamondBack non-slip vented aluminum stair treads mounted to underbody using Delron plastic slides for corrosion resistance. Step slide shall be securely held in both out and stored position, utilizing a heavy duty pneumatic cylinder designed to have an over center location which will assist the step in both extension and retraction. Each step shall be designed to hold 500 lbs.
- One (1) OnScene 9" Night Axe white LED ground light(s) shall be provided below the body. Light(s) shall be switchable but activated automatically when the park brake is set.
- Two (2) 3-1/2" x 3-1/2" black plastic louvered vents shall be provided in the lower compartment.

### **CURBSIDE COMPARTMENT - FRONT (C1)**

The interior useable compartment width shall be approximately 56.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 50.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

### **COMPARTMENT LAYOUT**

- There shall be vertically mounted aluminum Shelf-Trac welded to compartment walls for specified component installation. Shelf-Trac extrusion shall have side extruded channels for use in mounting or securing special ancillary items, without need for drilling into body.
- There shall be one (1) adjustable shelf/shelves approximately 24" deep. Each shelf shall be fabricated from 3/16" 3003 aluminum sheet with a 2" vertical flange along the front and rear edge.
  - Any equipment mounting on adjustable shelf shall be provided by Riverside County Fire Department after delivery.
  - The above component(s) shall have a smooth un-painted finish.
  - 3M™ Diamond Grade™ Conspicuity striping shall be provided on the front face of the shelf(s).
- This reflective stripe shall be red/white in color.

- There shall be one (1) adjustable shelf/shelves approximately 47" deep. Each shelf shall be fabricated from 3/16" 3003 aluminum sheet with a 2" vertical flange along the front and rear edges.

#### Riverside County Fire Department

- Any equipment mounting on adjustable shelf shall be provided by Riverside County Fire Department after delivery.
- The above component(s) shall have a smooth un-painted finish.
- 3M™ Diamond Grade™ Conspicuity striping shall be provided on the front face of the shelf(s).
- This reflective stripe shall be red/white in color.
- There shall be one (1) 400 lbs. slide-out tray(s) approximately 24" deep and as wide as the compartment layout or door opening permits. The tray top shall be fabricated from 3/16" 3003 aluminum sheet with a 3" vertical lip and welded corners to form a box type tray surface. The sliding tracks shall extend 100% of the slide length. The tray assembly shall utilize a pneumatic cylinder mounted on underside to hold the tray in both the extended and closed positions.
  - Equipment mounting on slide tray shall be:  
**SVI supplied Uline Big Wheel Handi Movers with pneumatic wheels Model# H-2176**
  - The above component(s) shall have a smooth un-painted finish.
- 3M™ Diamond Grade™ 2" wide conspicuity striping shall be provided on the front and side faces of the tray.
- This reflective stripe shall be red/white in color.
- There shall be one (1) OnScene Solutions 84 series slide-out, drop-down style aluminum tray base with 90% extension, and rating of 250 lbs. Slide-out tray(s) base shall be approximately **24"** deep and as wide as the compartment layout or door opening permits. It shall be located above the level of the chassis frame rails and shall be vertically adjustable in height. Each slide shall have a cable operated, spring loaded latch complimented by a large hand opening and red pull handle (Pull to Release) which will hold the tray in the closed position.
- Each tray shall be fabricated from 3/16" 3003 aluminum sheet and shall have welded corners to form a box type tray surface with an internal depth of approximately 3 ½".
  - The above component(s) shall have a smooth un-painted finish.
  - Any equipment mounting on slide tray shall be provided by Riverside County Fire Department after delivery.

#### Reflective Stripe: Tray Options, Red/White

- The floor of the compartment above the frame rails shall cover the area directly above the frame rails ONLY (non-extended floor).
- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.

The pendant for the cab tilt control shall be stored in a small open top storage box installed on the front wall of this compartment.

- There shall be one (1) underbody slide-out step. Step surface shall be constructed from 9" deep DiamondBack non-slip vented aluminum stair treads mounted to underbody using Delron plastic slides for corrosion resistance. Step slide shall be securely held in both out and stored position, utilizing a heavy duty pneumatic cylinder designed to have an over center location which will assist the step in both extension and retraction. Each step shall be designed to hold 500 lbs.
- One (1) OnScene 9" Night Axe white LED ground light(s) shall be provided below the body. Light(s) shall be switchable but activated automatically when the park brake is set.

### **REHAB WATER SYSTEM**

The apparatus shall be provided with an approximate one hundred (100) gallon UPF poly fresh water tank with an internal divider to separate the tank into one (1) approximate 60 gallon tank and one (1) approximate forty (40) gallon tank. The tank shall be securely mounted in the upper interior area of the compartment above the level of the frame rails per the sales drawing. The tank shall be filled from the fill valve located behind the hinged access door below the bathroom compartment and designed such that the top area of the water tank is open between the inner chambers allowing both portions of the water tank to be filled simultaneously. A 1" over flow tube shall be plumbed to a location below frame rails.

The tank shall be plumbed to a Shurflo 12 VDC electric pump system of sufficient size to provide 40 psi at outlets located in rear wheel well fender panels.

### **HOSE OUTLETS (Utilize Pex and Sharkbite Fittings)**

Two (2) 3/4" garden hose outlets will be provided, one (1) each side of rear fender panels. The outlets shall be located behind a Cast Product hinged door panel. Each outlet shall be equipped with a 1/4 turn shut-off valve.

The plumbing to the hose outlets from the tank and to the pump shall be 1/2" flexible PVC water line. All plumbing shall be secured and protected to prevent damage for a mobile application.

## **CURBSIDE COMPARTMENT - AHEAD OF REAR WHEEL (C2)**

The interior useable compartment width shall be approximately 41.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 35.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

## **COMPARTMENT LAYOUT**

- There shall be vertically mounted aluminum Shelf-Trac welded to compartment walls for specified component installation. Shelf-Trac extrusion shall have side extruded channels for use in mounting or securing special ancillary items, without need for drilling into body.
- There shall be three (3) adjustable shelf/shelves approximately 24" deep. Each shelf shall be fabricated from 3/16" 3003 aluminum sheet with a 2" vertical flange along the front and rear edge.
  - Any equipment mounting on adjustable shelf shall be provided by Riverside County Fire Department after delivery.
  - The above component(s) shall have a smooth un-painted finish.
  - 3M™ Diamond Grade™ Conspicuity striping shall be provided on the front face of the shelf(s).
- This reflective stripe shall be red/white in color.

- **One (1) American Airworks PopCan™ - single unit, Class 4 fill station, part # AC70020 with dimensions of 12" x 12" x 24", and weight of 55 pounds shall be provided with completed unit.**

**SVI Trucks will add handles and wheels to this unit prior to installation on the completed vehicle.**

- The floor of the compartment above the frame rails shall cover the area directly above the frame rails ONLY (non-extended floor).
- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.
- There shall be one (1) underbody slide-out step. Step surface shall be constructed from 9" deep DiamondBack non-slip vented aluminum stair treads mounted to underbody using Delron plastic slides for corrosion resistance. Step slide shall be securely held in both out and stored position, utilizing a heavy duty pneumatic cylinder designed to have an over center location which will assist the step in both extension and retraction. Each step shall be designed to hold 500 lbs.
- One (1) OnScene 9" Night Axe white LED ground light(s) shall be provided below the body. Light(s) shall be switchable but activated automatically when the park brake is set.
- Two (2) 3-1/2" x 3-1/2" black plastic louvered vents shall be provided in the lower compartment.



### **CURBSIDE COMPARTMENT - ABOVE REAR WHEEL (C3)**

The interior useable compartment width shall be approximately 64.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 58.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

### **COMPARTMENT LAYOUT**

- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.
- Specified breathing air compressor and air storage system in center of compartment.

### **CURBSIDE COMPARTMENT - REAR (C4)**

The interior useable compartment width shall be approximately 64.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 58.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**

- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

#### **COMPARTMENT LAYOUT**

- There shall be vertically mounted aluminum Shelf-Trac welded to compartment walls for specified component installation. Shelf-Trac extrusion shall have side extruded channels for use in mounting or securing special ancillary items, without need for drilling into body.
- There shall be four (4) adjustable shelf/shelves approximately 12" deep. Each shelf shall be fabricated from 3/16" 3003 aluminum sheet with a 2" vertical flange along the front and rear edges.
  - Any equipment mounting on adjustable shelf shall be provided by Riverside County Fire Department after delivery.
  - The above component(s) shall have a smooth un-painted finish.
  - 3M™ Diamond Grade™ Conspicuity striping shall be provided on the front face of the shelf(s).
- This reflective stripe shall be red/white in color.
- There shall be one (1) vertical compartment partition(s) provided dividing the compartment into fore and aft sides. The vertical partition(s) shall be 3/16" (.188) 3003H-14 alloy smooth aluminum sheet. Partition shall be approximately Fill In from forward wall of compartment.
  - Partition shall be bolted in position at base and top of partition.
  - The above component(s) shall have a smooth un-painted finish.
- There shall be one (1) bolt-in vertical compartment partition(s) provided dividing a transverse compartment into streetside and curbside. The vertical partition(s) shall be 3/16" (.188) 3003H-14 alloy smooth aluminum sheet.
  - The above component(s) shall have a smooth un-painted finish.

- There shall be one (1) SCBA cylinder storage module for 7-5/8" OD (maximum) SCBA bottles. Each PVC tube shall be capable of storing two (2) cylinders, end-to-end. The module shall have an exterior shell fabricated from 1/8" (.125) 3003H-14 aluminum alloy sheet. The module shall have a 2" slope, front to back to prevent cylinders from sliding out. The SCBA cylinder storage tubing shall be fabricated from PVC pipe to resist damage or abrasion to cylinders. In addition there shall be rubber pad provided in the base of each storage tube for bottle protection and to resist slipping.
  - The SCBA cylinder module shall hold sixteen (16) individual 7-5/8" diameter PVC tubes with a capacity of (2) SCBA cylinders per tube.
- One (1) Lista drawer cabinet, model **ES450-RG-IDL-LG** shall be provided in compartment. The Lista cabinet shall be x **21.6" high, 34.25" wide, 22.5" deep**. Cabinet shall have four (4) individual locking drawers . The cabinet shall be Light Gray in color.
- The floor of the compartment above the frame rails shall cover the area directly above the frame rails ONLY (non-extended floor).
- One (1) Hannay ECR1618-17-18 electric cable reel(s) capable of storing 200' of 10/3 electric cable. Reel(s) shall be designed to hold 110% of the capacity of cord length, with fully enclosed 45 amp, three (3) conductor collector rings. Reel(s) shall be mounted to channel structure that allows for side-to-side adjustment of reel position.
  - Power rewind control(s) shall be in a position where the operator can observe the rewinding operation and not be more than 72 in. (1830 mm) above the operator's standing position, and shall be marked with a label indicating its function and shall be guarded to prevent accidental operation.
  - A label shall be provided in a visible location adjacent to reel with following information: Current rating, Current type, Phase, Voltage, and Total cord length.
    - The cable reel shall equipped with 200' of 10/3 SEOWW black cable, a molded plastic ball clamp, and a single heavy duty L5-30 twist-lock female plug at the end.
- One (1) Akron model EJBX series, cast aluminum electrical power distribution box with gray powder coat painted finish shall be provided. The power distribution box shall meet all requirements described in NFPA 1901. The power distribution box shall include the following outlets mounted on a backlit face plate;
  - A 12" pigtail that terminates in an L5-30 configuration to match the cable on the cord reel. The outlet configuration shall include:
    - One (1) 120 VAC, 5-20 duplex straight-blade receptacle
    - One (1) 120 VAC, 5-20 duplex straight-blade receptacle
    - One (1) 120 VAC, L5-20 single twist lock receptacle.
    - One (1) 120 VAC, L5-20 single twist lock receptacle.
- One (1) Akron Brass model EJB-VMT aluminum treadplate vertical mounting bracket for specified power distribution box shall be provided and mounted in compartment per Riverside County Fire Department.
- The fairlead roller shall be mounted directly to the reel.

- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.
- There shall be one (1) 120 VAC outlet(s) located in compartment.
  - The outlet receptacle(s) shall be 20 amp, straight-blade (NEMA 5-20R).
  - Outlet(s) shall be powered by both the on-board generator and shore power system through a relay system.
  - The outlet shall be located on forward wall, upper left area.
- There shall be one (1) underbody slide-out step. Step surface shall be constructed from 9" deep DiamondBack non-slip vented aluminum stair treads mounted to underbody using Delron plastic slides for corrosion resistance. Step slide shall be securely held in both out and stored position, utilizing a heavy duty pneumatic cylinder designed to have an over center location which will assist the step in both extension and retraction. Each step shall be designed to hold 500 lbs.
- One (1) OnScene 9" Night Axe white LED ground light(s) shall be provided below the body. Light(s) shall be switchable but activated automatically when the park brake is set.
- Two (2) 3-1/2" x 3-1/2" black plastic louvered vents shall be provided in the lower compartment.

## **REAR COMPARTMENT - CENTER (RC1)**

The rear center compartment shall be closed to both side rear compartments.

The rear center compartment shall begin just above the bumper height and be as high as the side compartments, unless specified otherwise. The body sub-frame shall extend at least 20" into the compartment to allow for the spring loaded body mounts.

The interior useable compartment space shall be approximately 70.5" wide.

- This compartment shall have an Amdor roll-up door.
- The compartment door opening shall be approximately 64.0" wide.
- The roll-up door slats and the door track components shall be painted to match the single tone exterior color. The painted roll-up doors shall be equipped with Extended Slat Shoe (ESS) feature which eliminates abrasion on the door finish.  
**Doors will have Anodized tracks.**
- The Amdor door shall be equipped with an integral switch in the lower door handle retainer block to activate compartment lighting and door ajar signal in cab when door is opened.
- A keyed 1250 cylinder lock shall be provided on bottom rail of the roll-up door.
- The roll-up doors shall be manually operated with a key.
- One (1) 1" wide nylon strap shall be provided to assist in closing the compartment door. The strap shall be fastened to the lower left inside door sill with a nickel plated Footman loop secured to back of door. The strap shall extend from door to a nickel plated Footman loop secured to wall or vertical slot of Shelf-Trac on left side of the door opening.
- One (1) aluminum drip pan/door guard shall be provided below door roll area. Drip pan/door guard shall have thumb nuts making it easily removable without tools with a maintenance-free, un-painted finish. A plastic drain line shall be provided on each end of the drip pan to lower door threshold.
- Compartment threshold protection shall be provided on the bottom edge of the compartment door sill. The threshold protection shall be an extruded aluminum shape with an un-painted anodized finish.

## **COMPARTMENT LAYOUT**

- There shall be vertically mounted aluminum Shelf-Trac welded to compartment walls for specified component installation. Shelf-Trac extrusion shall have side extruded channels for use in mounting or securing special ancillary items, without need for drilling into body.

**Shelf track will be above the Fill Station for Adjustable shelf.**

- There shall be one (1) adjustable shelf/shelves approximately 20" deep. Each shelf shall be fabricated from 3/16" 3003 aluminum sheet with a 2" vertical flange along the front and rear edges.
  - Any equipment mounting on adjustable shelf shall be provided by Riverside County Fire Department after delivery.

- The above component(s) shall have a smooth un-painted finish.
- 3M™ Diamond Grade™ Conspicuity striping shall be provided on the front face of the shelf(s).
- This reflective stripe shall be red/white in color.
- One (1) Hannay EFH1516-17-18 high pressure air hose reel(s) shall be provided in this compartment. Reel shall be designed to hold 110% of the capacity needed.
  - Power rewind control(s) shall be in a position where the operator can observe the rewinding operation and not be more than 72 in. (1830 mm) above the operator's standing position, and shall be marked with a label indicating its function and shall be guarded to prevent accidental operation.
  - A label shall be provided in a visible location adjacent to reel with following information: (1) Utility air or breathing air, (2) Operating pressure, (3) Total hose length, (4) Hose size (ID).
  - The hose reel shall be equipped with 300' of 3/16" Parker 527BA 7,000 PSI, high pressure air hose. A molded plastic ball clamp shall be provided on the hose to stop it at the 4-way roller. The hose shall be Blue in color with a red color coded end. High pressure air hose and couplings are to have a pressure rating equal to or greater than the highest pressure expected to be encountered, with a safety factor of 4 to 1.
  - The fitting on the end of the high pressure air hose reel shall be a CGA-347 high pressure fitting.
  - The air supply shall be from the specified mobile breathing air system.
  - The air supply for specified reel(s) shall be from the on-board specified mobile breathing air system. The reel shut-off valve, pressure regulator, and gauge shall be provided at the specified breathing air control panel, not exceeding 72" from ground.
- The fairlead roller shall be mounted directly to the reel.

#### **COMMUNICATION SPEAKER INSTALLATION**

**There shall be one (1) MIS8C mobile communication speaker with a compact flush mount design supplied and installed in this compartment.**

**A twist-knob volume regulator shall also be supplied and installed in a position easily accessible for the operator to control the sound output.**

**Signal wire shall be supplied to the speaker and terminate in the area behind the officer's seat in the cab.**

**MODEL: MIS8C**

**Wattage: 10**

**Frequency Response: 900 Hz 6.3 kHz**

**Impedance: 8 Ohms**

**Sensitivity: 101 dB SPL, 1W**

**Dimensions: 5.5" Diameter x 4.2" Deep**

**Color: Gray**

**There shall be a Kemo Amplifier M032S for this speaker with separate volume control.**

**Both speaker and amp will be located by the fill station.**

- Two (2) OnScene Access PRO white LED, full height compartment lights, vertically mounted.
- Two (2) Bauer model CFS5.5 2M NFPA 1901 compliant containment type two (2) cylinder filling stations, one (1) with compressor controls rated for cylinder pressures up to 5,500 PSI shall be provided with proper reinforcement for weight of fill stations and venting thru floor opening. Fill stations together will be approximately 65" wide x 50.25" high x 21" deep, and weigh approximately 1,726 lbs. High pressure air hose and couplings are to have a pressure rating equal to or greater than the highest pressure expected to be encountered, with a safety factor of 4 to 1.
  - Filling operation shall be controlled with manual controls mounted on front of fill station. An air flow selector valve to fill from either compressor or storage, and manual valves and gauges for each air storage cylinder (maximum of four (4)).
  - An air storage refill port shall be provided on the fill station.
- There shall be a 25' 7000psi refill hose supplied with the apparatus for connection between a station/facility compressor and the fill station/storage refill port.
  - The fill station fill whip(s) shall terminate in a high pressure CGA-347 threaded connectors for 4,500 - 5,500 PSI air pack cylinders.
  - The fill station(s) shall be protected by a 6,000 psi relief valve.

## **BODY OPTIONS AND UPGRADES**

### **PLASTIC FLOOR AND SHELF TILE**

Turtle Plastics 12" x 12" x 1/2", self-draining plastic inter-locking material shall be cut to size and cover all compartment floors, shelves, and trays.

- The plastic floor tile shall be black.
- The plastic edge trim shall be **Yellow**.

### **ROOF ACCESS HANDRAIL**

There shall be one(1) Hansen International 24" x 1-1/8" vertical handrail on **roof of** body. Handrail shall be NFPA compliant formed from anodized aluminum with knurled anti-slip finish.

Handrail shall be back-lit with a Safetylite, 12 VDC white LED light tube. Lights shall be activated with headlight and park brake set circuits.

A safety sign FAMA23, which warns of the proper climbing method, shall be visible to personnel entering the cab and at each designated climbing location on the body.

A safety sign FAMA24, which warns personnel not to ride on the vehicle, shall be located at the rear step areas and at any cross walkways.

### **FOLDING STEP(S)**

There shall be five (5) Innovative Controls polished cast aluminum folding step(s) provided and installed on completed vehicle. Each step shall be heavy duty with stainless steel spring and textured step surface meeting NFPA standards. **Customer wants to make sure that these will have the light in them.**

### **ROLL-OUT AWNING STREETSIDE**

A Carefree Mirage, 110 Volt AC powered, Lateral Arm Acrylic Patio Awning with Direct Response Electronics shall be installed on the body. The Direct Response Electronics includes easy-to-use controls and a Motion Detection System. The awning shall have a system to detect canopy motion, the most important element to prevent wind/weather damage. The awning shall automatically retract when the canopy reaches a certain level of movement, you determine the movement level on the control panel.

The 110V motor shall be completely sealed and UL approved. The awning pitch shall be adjusted to up to 30"

The awning shall be 14' long with a 10' projection, (size refers to box length; actual fabric length will be 8" shorter.)

The Mirage shall be covered by a "Two and Four" Limited Warranty - Two years 100% parts, labor, & freight on canopy, four years 100% parts, labor, and freight on motor, electronics, roller & hardware. Warranty covers manufacturer's defects only. Wind and rain damage are not covered.

A red flashing or rotating light located in the driving compartment shall be illuminated automatically whenever the vehicles parking brake is not fully engaged, indicating that the awning is not in stowed position, as required by NFPA 1901.



- The Firesist HUV awning fabric color shall be crimson red (#88003-000).

The specified awning above shall be recess mounted into upper body side. An aluminum box enclosure shall be fabricated and recessed into upper body side for awning mounting and painted same color as upper body. The recessed awning shall add approximately 1.5" to body width.

#### **AWNING HOUSING COLOR**

The awnings standard white housing color shall be re-painted to match upper body color.

#### **ROLL-OUT AWNING CURBSIDE**

A Carefree Mirage, 110 Volt AC powered, Lateral Arm Acrylic Patio Awning with Direct Response Electronics shall be installed on the body. The Direct Response Electronics includes easy-to-use controls and a Motion Detection System. The awning shall have a system to detect canopy motion, the most important element to prevent wind/weather damage. The awning shall automatically retract when the canopy reaches a certain level of movement, you determine the movement level on the control panel.

The 110V motor shall be completely sealed and UL approved. The awning pitch shall be adjusted to up to 30"

The awning shall be 14' long with a 10' projection, (size refers to box length; actual fabric length will be 8" shorter.)

The Mirage shall be covered by a "Two and Four" Limited Warranty - Two years 100% parts, labor, & freight on canopy, four years 100% parts, labor, and freight on motor, electronics, roller & hardware. Warranty covers manufacturer's defects only. Wind and rain damage are not covered.

A red flashing or rotating light located in the driving compartment shall be illuminated automatically whenever the vehicles parking brake is not fully engaged, indicating that the awning is not in stowed position, as required by NFPA 1901.

- The Firesist HUV awning fabric color shall be crimson red (#88003-000).

The specified awning above shall be recess mounted into upper body side. An aluminum box enclosure shall be fabricated and recessed into upper body side for awning mounting and painted same color as upper body. The recessed awning shall add approximately 1.5" to body width.

#### **AWNING HOUSING COLOR**

The awnings standard white housing color shall be re-painted to match upper body color.

### **REAR ROLL-OUT AWNING**

The upper rear of truck shall be equipped with a Carefree Ltd Freedom wall mount awning. The box the awning is stored in is approximately 8' wide x 5-3/8" high x 5" deep and white in color. The awning shall be 8' wide with an extension length of 6-1/2'. The awning support arms are hidden inside the lead rail. The awning will be extended and retracted using a 12VDC motorized system with a manual override if power is lost.

A red flashing or rotating light located in the driving compartment shall be illuminated automatically whenever the vehicles parking brake is not fully engaged, indicating that the awning is not in stowed position, as required by NFPA 1901.

- The Firesist HUV awning fabric color shall be crimson red (#88003-000).

The specified awning above shall be surface mounted to upper body side. The awning shall add approximately 5.75" to body width.

### **AWNING HOUSING COLOR**

The awnings standard white housing color shall be re-painted to match upper body color.

### **AWNING LED LIGHTS**

The specified awning shall be provided with white LED lights under lead rail. Lights shall be turned on automatically when awning is extended, and turned off when awning is stowed.

### **ROOF ACCESS HATCH COVER**

One (1) roof access hatch cover shall be provided in the roof structure to allow for installation or removal of large equipment into the compartment area. The roof around the hatch opening shall be reinforced as necessary to prevent deflection in the roof area. The hatch cover shall overlap a 2" vertical lip on the body roof to resist entry of moisture. It shall be sealed with automotive type rubber molding to provide a weather resistant seal.

The hatch cover shall have a lift-up type door hinged on the front side. The door shall be fabricated from 3/16" aluminum treadplate with a pair of pneumatic type cylinders mounted to hold the door in the open position. The door shall be mounted using a full length 14 gauge stainless steel hinge, with 1/4" stainless steel pin. A polyester barrier film gasket shall be placed between the stainless steel hinge and any dissimilar metals as necessary to resist corrosion.

## **LOW VOLTAGE ELECTRICAL SYSTEM- 12 VDC**

### **General**

Any low voltage electrical systems or warning devices installed on the fire apparatus shall be appropriate for the mounting location and intended electrical load.

Where wire passes through sheet metal, grommets shall be used to protect wire and wire looms. Electrical connections shall be with double crimp water-tight heat shrink connectors.

All 12 VDC wiring running from front to back of vehicle body shall be run in full length electrical wiring raceway down each side of body.

### **Wiring**

All electrical circuit feeder wiring supplied and installed by the fire apparatus manufacturer shall meet the requirements of NFPA Chapter 13.

The circuit feeder wire shall be stranded copper or copper alloy conductors of a gauge rated to carry 125% of the maximum current for which the circuit is protected. Voltage drops in all wiring from the power source to the using device shall not exceed 10%. The use of star washers for circuit ground connections shall not be permitted.

All circuits shall otherwise be wired in conformance with SAE J1292, *Automobile, Truck, Truck-Tractor, Trailer, and Motor Coach Wiring*.

### **Wiring and Wire Harness Construction**

All insulated wire and cable shall conform to SAE J1127, *Low Voltage Battery Cable*, or SAE J1128, *Low Voltage Primary Cable*, type SXL, GXL, or TXL.

All conductors shall be constructed in accordance with SAE J1127 or SAE J1128, except where good engineering practice dictates special strand construction. Conductor materials and stranding, other than copper, shall be permitted if all applicable requirements for physical, electrical, and environmental conditions are met as dictated by the end application. Physical and dimensional values of conductor insulation shall be in conformance with the requirements of SAE J1127 or SAE J1128, except where good engineering practice dictates special conductor insulation. The overall covering of conductors shall be moisture-resistant loom or braid that has a minimum continuous rating of 194°F (90°C) except where good engineering practice dictates special consideration for loom installations exposed to higher temperatures. The overall covering of jacketed cables shall be moisture resistant and have a minimum continuous temperature rating of 194°F (90°C), except where good engineering practice dictates special consideration for cable installations exposed to higher temperatures.

All wiring connections and terminations shall use a method that provides a positive mechanical and electrical connection. The wiring connections and terminations shall be installed in accordance with the device manufacturer's instructions. All ungrounded electrical terminals shall have protective covers or be in enclosures. Wire nut, insulation displacement, and insulation piercing connections shall not be used.

Wiring shall be restrained to prevent damage caused by chafing or ice buildup and protected against heat, liquid contaminants, or other environmental factors.

Wiring shall be uniquely identified at least every 2 ft (0.6 m) by color coding or permanent marking with a circuit function code. The identification shall reference a wiring diagram.

Circuits shall be provided with properly rated low voltage over-current protective devices. Such devices shall be readily accessible and protected against heat in excess of the over-current device's design range, mechanical damage, and water spray. Circuit protection shall be accomplished by utilizing fuses, circuit breakers, fusible links, or solid state equivalent devices.

If a mechanical-type device is used, it shall conform to one of the following SAE standards:

- 1) SAE J156, *Fusible Links*
- 2) SAE J553, *Circuit Breakers*
- 3) SAE J554, *Electric Fuses (Cartridge Type)*
- 4) SAE J1888, *High Current Time Lag Electric Fuses*
- 5) SAE J2077, *Miniature Blade Type Electrical Fuses*

Switches, relays, terminals, and connectors shall have a direct current (dc) rating of 125% of maximum current for which the circuit is protected.

#### Power Supply

A 12 V or greater electrical alternator shall be provided. The alternator shall have a minimum output at idle to meet the minimum continuous electrical load of the vehicle, at 200°F (93°C) ambient temperature within the engine compartment, and shall be provided with full automatic regulation.

#### Minimum Continuous Electrical Load

The minimum continuous electrical load shall consist of the total amperage required to simultaneously operate the following in a stationary mode during emergency operations:

- 1) The propulsion engine and transmission
- 2) All legally required clearance and marker lights, headlights, and other electrical devices except windshield wipers and four-way hazard flashers
- 3) The radio(s) at a duty cycle of 10 percent transmit and 90% receive (for calculation and testing purposes, a default value of 5 A continuous)
- 4) The lighting necessary to produce 2 fc (20 lx) of illumination on all walking surfaces on the apparatus and on the ground at all egress points onto and off the apparatus, 5 fc (50 lx) of illumination on all control and instrument panels, and 50 percent of the total compartment lighting loads
- 5) The minimum optical warning system, where the apparatus is blocking the right-of way
- 6) The continuous electrical current required to simultaneously operate any fire pumps, aerial devices, and hydraulic pumps
- 7) Other warning devices and electrical loads defined by the purchaser as critical to the mission of the apparatus

If the apparatus is equipped to tow a trailer, an additional 45 A shall be added to the minimum continuous electrical load to provide electrical power for the federally required clearance and marker lighting and the optical warning devices mounted on the trailer.

The condition of the low voltage electrical system shall be monitored by a warning system that provides both an audible and a visual signal to persons on, in, or near the apparatus of an impending electrical system failure caused by the excessive discharge of the battery set.

The charge status of the battery shall be determined either by direct measurement of the battery charge or indirectly by monitoring the electrical system voltage.

If electrical system voltage is monitored, the alarm shall sound if the system voltage at the battery or at the master load disconnect switch drops below 11.8 V for 12 V nominal systems, 23.6 V for 24 V nominal systems, or 35.4 V for 42 V nominal systems for more than 120 seconds.

A voltmeter shall be mounted on the driver's instrument panel to allow direct observation of the system voltage.

#### Electromagnetic Interference

Electromagnetic interference suppression shall be provided, as required, to satisfy the radiation limits specified in SAE J551/1, *Performance Levels and Methods of Measurement of Electromagnetic Compatibility of Vehicles, Boats (up to 15 m), and Machines (16.6 Hz to 18 GHz)*.

#### Wiring Diagram

A complete electrical wiring schematic of actual system shall be provided with finished apparatus. Similar or generic type electrical schematics shall NOT BE ACCEPTABLE.

#### Low Voltage Electrical System Performance Test

A low voltage electrical system test certification shall be provided with delivered apparatus.

### **12 VOLT MULTIPLEX CONTROL CENTER**

The apparatus shall be equipped with a Weldon V-MUX multiplexed 12 volt electrical system that will provide complete diagnostic capability, No Exception. The system shall have the capability of delivering multiple signals via a CAN bus, utilizing specifications set forth by SAE J1939. The system shall be node based to maximize stability so that failure of one node does not affect the operation of the other nodes. The system shall use shielded twisted-pair wire for transmission of system function signals. The shielded wire shall provide protection against EMI and RFI noise interruptions.

The multiplex system shall be responsible for providing power management functions as well as load shedding. The warning light system shall be controlled by the multiplex system. The system shall be capable of displaying text and/or graphic messages on a display module. The system shall be based on solid-state technology and shall include self-contained diagnostic indicators.

#### **WELDON CERTIFICATION**

A letter shall be provided with bid submittal that the Contractor has successfully completed the Weldon training requirements for Level 1 of the V-MUX Certified Supplier Program and is authorized to design, build, and service V-MUX electrical systems.

The apparatus shall be equipped with a Weldon V-MUX multiplexed 12 volt electrical system that will provide complete diagnostic capability, No Exception. The system shall have the capability of delivering multiple signals via a CAN bus, utilizing specifications set forth by SAE J1939. The system shall be node based to maximize stability so that failure of one node does not affect the operation of the other nodes. The system shall use shielded twisted-pair wire for transmission of system function signals. The shielded wire shall provide protection against EMI and RFI noise interruptions.

The multiplex system shall be responsible for providing power management functions as well as load shedding. The warning light system shall be controlled by the multiplex system. The system shall be capable of displaying text and/or graphic messages on a display module. The system shall be based on solid-state technology and shall include self-contained diagnostic indicators.

## **MULTIPLEX SYSTEM INTERFACE DISPLAY**

The Weldon V-MUX Vista IV multiplex system interface display(s) shall be provided by the cab/chassis manufacturer. The full-color Vista interface display allows the user to control warning and scene lighting, HVAC controls (when specified), and view on-board diagnostics including service information. This display has a wide operating temperature range, automatic screen switching in response to current conditions, and a sleep mode option to eliminate night glare. The following features shall be included;

- 800 x 480 resolution
- Four video ports
- Flash updates with USB memory stick
- Display inside and outside temperature (when specified)
- Automatic climate control (when specified)
- 100% Configurable (OEM Level)
- Field re-programmable
- Peer to peer network
- On-board diagnostics / service information
- Colors change to indicate button status
- Video Ready for: Backup camera, Thermal camera, DVD, GPS...

## **BATTERY SYSTEM**

Any body builder supplied battery connections shall be heavy duty type with cables terminating in heat shrink loom. Heavy duty battery cables shall provide maximum power to the electrical system. Where required, the cables shall be shielded from exhaust tubing and the muffler. Large rubber grommets shall be provided where cables enter the battery compartment.

Where an enclosed battery compartment is provided, it shall be ventilated to the exterior to prevent the buildup of heat and explosive fumes. The batteries shall be protected against vibration and temperatures that exceed the battery manufacturer's recommendation.

## **BATTERY SWITCH**

One (1) battery disconnect switch shall be provided in cab located within easy reach of driver with green indicator light that is visible from the driver's position. The switch and indicator light shall be supplied and installed by the cab/chassis manufacturer.

## **BATTERY SOLENOID**

Battery switch shall consist of a minimum 200 ampere, constant duty solenoid to feed from positive side of battery.

## **SHORE POWER INLET**

**Chassis supplied AC, and electrical Inlet with Blue cover will be wired to a transfer switch done by SVI.**

## **BATTERY CONDITIONER**

The battery conditioner shall be supplied and installed by the cab chassis manufacturer.

### **ENGINE COMPARTMENT LIGHT**

Engine compartment light(s) shall be supplied and installed by the cab chassis manufacturer.

### **CAB HAZARD WARNING LIGHT**

A red flashing or rotating light, located in the driving compartment. The light shall be furnished by the cab/chassis manufacturer. The light shall be illuminated automatically whenever the vehicles parking brake is not fully engaged and any of the following conditions exist:

- Any passenger or equipment compartment door is not closed.
- Any ladder or equipment rack is not in the stowed position.
- Stabilizer system is not in its stowed position.
- Powered light tower is not stowed.
- Any other device permanently attached to the apparatus is open, extended, or deployed in a manner that is likely to cause damage to the apparatus if the apparatus is moved.

Compartments and equipment meeting all of the following conditions shall be permitted to be exempt from being wired to the hazard light:

- The volume is less than or equal to 4 ft<sup>3</sup> (0.1 m<sup>3</sup>).
- The compartment has an opening less than or equal to 144 in.<sup>2</sup> (92,900 mm<sup>2</sup>).
- The open door does not extend sideways beyond the mirrors or up above the top of the fire apparatus.
- All equipment in the compartment is restrained so that nothing can fall out if the door is open while the apparatus is moving.
- Manually raised pole lights with an extension of less than 5 ft (1.5 m).

The hazard light shall be labeled "DO NOT MOVE APPARATUS WHEN FLASHING".

### **BACK-UP ALARM**

An electronic back-up alarm shall be supplied and installed by the cab/chassis manufacturer. The back-up alarm shall actuate automatically when the transmission gear selector is placed in reverse.

### **BODY MOUNTED 360 CAMERAS**

The cab chassis provided three (3) FRC Seon series 360 cameras shall be installed on the sides and rear of the body. Camera system shall be calibrated and operational upon delivery.

### **INTERIOR LED LIGHTS**

One (1) OnScene Solution model #70156, 10" x 10" x 7/8", 10-30 VDC, surface mount dual red and white LED light(s) with clear lens shall be provided throughout the vehicle. In addition light(s) will be capable of a five (5) second delay after switching off.

The light(s) shall be switched with high/low intensity setting at the entry door(s). An Innovative Controls black back-lit switch panel shall be provided to control specified lighting or other control switching.

**NOTE: The cab and rehab area lights will be centered.**

### **INTERIOR LIGHT SWITCH**

- There shall be One (1) interior light switch panel located on the curbside, forward bulkhead wall.

### **TAIL LIGHTS**

Rear body tail lights shall be vertically mounted and located per Federal Motor Vehicle Safety Standards, FMVSS and Canadian Motor Vehicle Safety Standards CMVSS. The following lights shall be furnished;

- Two (2) Federal amber LED QL64Z-ARROW turn signal lights
- Two (2) Federal red LED QL64Z-BTT stop/tail lights
- Two (2) Federal white LED QL64Z-BACKUP back-up lights

Each light shall have a chrome flange.

### **MIDSHIP MARKER/TURN SIGNAL**

Two (2) Whelen model T0A00MAR 2" round amber LED midship body clearance marker/turn signal lights shall be provided and installed, one (1) light on each side of the body, in forward wheel well of rear axle. Midship marker/turn lights shall be wired to the headlight circuit of the chassis.

### **MARKER LIGHTS**

The body shall be equipped with all necessary side and rear clearance lights and reflectors in accordance with Federal Motor Vehicle Safety Standards (FMVSS) and Canadian Motor Vehicle Safety Standards (CMVSS). Clearance lights on body shall be connected to the clearance light circuit of the chassis.

### **CAB STEP LIGHTS / GROUND LIGHTS**

The step lights and/or ground lights shall be supplied and installed by the cab/chassis manufacturer.

### **LICENSE PLATE LIGHT**

One (1) Arrow #437 chrome plated LED license plate light shall be installed on the rear of the body. License plate light shall be wired to the headlight circuit of chassis. A fastener system shall be provided for license plate installation.

### **ELECTRONIC SIREN**

The siren control head shall be supplied by the cab/chassis manufacturer and **installed by SVI**, if required by Riverside County Fire Department. Siren power shall be wired through the master warning light switch.

The specified siren functions shall be configured by cab chassis manufacturer.



## **FRONT SCENE LIGHT(S)**

The following front scene lights shall be mounted on chassis brow above windshield.

**FRC two (2) mini brow lights with black housing model # FT-MB-15-FT-B;** roof mount light shall be installed. The lower mounting bracket shall allow the bottom of the lamphead to pivot and the upper mounting bracket shall extend out on a turnbuckle that is adjustable to set the lamphead angle. Wiring shall extend from a weatherproof strain relief at the rear of the lamphead.

Lamphead shall be provided with a lifetime warranty to original apparatus purchaser.

The lights shall be controlled at the multiplex display(s) in the cab.

## **SIDE SCENE LIGHTS**

There shall be four (4) Fire Research Spectra Max model SPA260-Q20 surface mount LED light(s) provided on the upper body. Light quantity shall be divided equally per side. The light(s) shall be mounted with four (4) screws to a flat surface. It shall be no more than 6" high by 14 1/2" wide and have a profile of less than 1 3/4" beyond the mounting surface. Wiring shall extend from the electronics box at the rear of the lamphead. Lamphead shall be provided with black powder coat finish.

The lamphead shall have sixty (60) ultra-bright white LEDs, 56 for flood lighting and 4 to provide a spot light beam pattern. It shall operate at 12 volts DC, draw 13.8 amps, and generate 20,000 lumens of light. The lamphead shall have a unique lens that directs flood lighting onto the work area and focuses the spot light beam into the distance.

The lights shall be controlled at the multiplex display(s) in the cab.

Floodlight housing shall be white with chrome bezel.

## **REAR SCENE LIGHTS**

There shall be two (2) Federal QuadraFlare model QL64LEDSCENE, 6" x 4" recess mounted LED scene lights provided on the upper rear body. Each light will have a clear lens and chrome bezel.

The above scene lights shall light to a level of at least 3 fc (30 lx), measured at 25 equally spaced points on a 2.5 ft (750 mm) grid within a 10 ft x 10 ft (3 m x 3m) square to the rear of vehicle.

The lights shall be controlled at the multiplex display(s) in the cab.

The rear scene lights shall also be activated when the apparatus is in reverse.

## **TRAFFIC DIRECTIONAL LIGHT**

One (1) Federal SignalMaster #MPSUSM42-BRK-30 42, seven (7) LED light, (6) Amber and (1) red, traffic directional warning device with 30' control cable shall be located on upper rear body. The control head shall be **through the VMUX and not through control head in dash panel.**

NOTE: Center red light will be a brake light

The traffic directional light shall be recess mounted into the upper rear body fabricated from 1/8" aluminum treadplate.

## **WARNING LIGHT PACKAGE**

Each apparatus shall have a system of optical warning devices that meets or exceeds the requirements of this section.

The optical warning system shall consist of an upper and a lower warning level. The requirements for each level shall be met by the warning devices in that particular level without consideration of the warning devices in the other level.

For the purposes of defining and measuring the required optical performance, the upper and lower warning levels shall be divided into four (4) warning zones. The four zones shall be determined by lines drawn through the geometric center of the apparatus at 45 degrees to a line drawn lengthwise through the geometric center of the apparatus. The four (4) zones shall be designated A, B, C, and D in a clockwise direction, with zone A to the front of the apparatus.

Each optical warning device shall be installed on the apparatus and connected to the apparatus's electrical system in accordance with the requirements of this standard and the requirements of the manufacturer of the device.

A master optical warning system switch that energizes all the optical warning devices shall be provided.

The optical warning system on the fire apparatus shall be capable of two (2) separate signaling modes during emergency operations. One (1) mode shall signal to drivers and pedestrians that the apparatus is responding to an emergency and is calling for the right-of-way. One (1) mode shall signal that the apparatus is stopped and is blocking the right-of-way. The use of some or all of the same warning lights shall be permitted for both modes provided the other requirements of this chapter are met.

A switching system shall be provided that senses the position of the parking brake or the park position of an automatic transmission. When the master optical warning system switch is closed and the parking brake is released or the automatic transmission is not in park, the warning devices signaling the call for the right-of-way shall be energized. When the master optical warning system switch is closed and the parking brake is on or the automatic transmission is in park, the warning devices signaling the blockage of the right-of-way shall be energized. The system shall be permitted to have a method of modifying the two (2) signaling modes.

The optical warning devices shall be constructed or arranged so as to avoid the projection of light, either directly or through mirrors, into any driving or crew compartment(s). The front optical warning devices shall be placed so as to maintain the maximum possible separation from the headlights.

Steadily burning, non flashing optical sources shall be permitted to be used.

## **UPPER LEVEL OPTICAL WARNING DEVICES**

The upper-level optical warning devices shall be mounted as high and as close to the corner points of the apparatus as is practical to define the clearance lines of the apparatus. The upper-level optical warning devices shall not be mounted above the maximum height, specified by the device manufacturer.

### **ZONE A - FRONT WARNING LIGHTS**

See Chassis Modification section for cab mounted warning lights.

The light bar shall be supplied and installed by the cab/chassis manufacturer.

The lightbar(s) shall be separately controlled at multiplex display(s) in the cab.

### **ZONE B & D - SIDE WARNING LIGHTS**

There shall be four (4) Federal Signal QL97 LED Light(s) provided, two (2) each side. The light head shall include twenty-six (26) programmable flash patterns and Hi/Lo intensities.

Each Light shall have:

- Red LEDs
- Clear Lens

Each light shall have a chrome flange.

- Flash Pattern shall be Federal Signal DoubleFlash 150 - Simultaneous

The lights shall be controlled at the multiplex display(s) in the cab.

### **ZONE C - REAR WARNING LIGHTS**

There shall be two (2) Federal Signal QL97 LED Light(s) provided, one (1) each side. The light head shall include twenty-six (26) programmable flash patterns and Hi/Lo intensities.

Each Light shall have:

- Red LEDs
- Clear Lens

Each light shall have a chrome flange.

- Flash Pattern shall be Federal Signal DoubleFlash 150 - Simultaneous

The lights shall be controlled at the multiplex display(s) in the cab.

## LOWER LEVEL OPTICAL WARNING DEVICES

To define the clearance lines of the apparatus, the optical center of the lower-level optical warning devices in the front of the vehicle shall be mounted on or forward of the front axle centerline and as close to the front corner points of the apparatus as is practical.

The optical center of the lower-level optical warning devices at the rear of the vehicle shall be mounted on or behind the rear axle centerline and as close to the rear corners of the apparatus as is practical. The optical center of any lower-level device shall be between 18 in. and 62 in. (460 mm and 1600 mm) above level ground for large apparatus, and 18 in. and 48 in. (460 mm and 1600 mm) above level ground.

A midship optical warning device shall be mounted right and the left sides of the apparatus if the distance between the front and rear lower-level optical devices exceeds 25 ft (7.6 m) at the optical center. Additional midship optical warning devices shall be required, where necessary, to maintain a horizontal distance between the centers of adjacent lower-level optical warning devices of 25 ft (7.6 m) or less. The optical center of any midship mounted optical warning device shall be between 18 in. and 62 in. (460 mm and 1600 mm) above level ground.

### ZONE A - FRONT WARNING LIGHTS, LOWER

The front lower warning lights shall be supplied and installed by the cab/chassis manufacturer. They shall be Federal lights to complete an NFPA compliant lower level warning light system.

The lights shall be controlled at the multiplex display(s) in the cab.

### ZONES B AND D - CAB INTERSECTOR LIGHT (CAB FRONT CORNERS)

The front lower warning lights shall be supplied and installed by the cab/chassis manufacturer. They shall be Federal lights to complete an NFPA compliant lower level warning light system.

The lights shall be controlled at the multiplex display(s) in the cab.

### ZONES B AND D - BODY LIGHT (BODY WHEELWELL AREA)

There shall be two (2) Federal Signal **Micropulse Ultra 12's (MPS121U-R)** light(s) provided, one (1) each side.

Each Light shall have:

- Red LEDs
- **Clear** Lens

Each light shall have a chrome flange.

- Flash Pattern shall be Federal Signal DoubleFlash 150 - Simultaneous

The lights shall be controlled at the multiplex display(s) in the cab.

#### ZONES B AND D - BODY INTERSECTOR LIGHT (BODY REAR CORNERS)

There shall be two (2) Federal Signal QL64 LED Light(s) provided, one (1) each side. The light head shall include twenty-six (26) programmable flash patterns and Hi/Lo intensities.

Each Light shall have:

- Red LEDs
- Clear Lens

Each light shall have a chrome flange.

- Flash Pattern shall be Federal Signal DoubleFlash 150 - Simultaneous

The lights shall be controlled at the multiplex display(s) in the cab.

#### ZONE C - REAR WARNING LIGHTS (LOWER REAR CORNERS)

There shall be two (2) Federal Signal QL64 LED Light(s) provided, one (1) each side. The light head shall include twenty-six (26) programmable flash patterns and Hi/Lo intensities.

Each Light shall have:

- Red LEDs
- Clear Lens

Each light shall have a chrome flange.

- Flash Pattern shall be Federal Signal DoubleFlash 150 - Simultaneous

The lights shall be controlled at the multiplex display(s) in the cab.

## **LINE VOLTAGE ELECTRICAL SYSTEM**

### **MARATHON PTO GENERATOR**

The vehicle shall be equipped with a Marathon harsh duty Magna Plus series, two (2) bearing generator system with a capacity of 40,000 watts at 120/240 or 120/208V VAC, 3-phase. Current frequency shall be stable at 60 hertz.

The transmission's PTO port and PTO, or the split shaft PTO, and all associated drive shaft components shall be rated to support the continuous duty torque requirements of the generator's continuous duty rating as stated on the power source nameplate.

Where the generator is driven by the chassis engine and transmission through a split shaft PTO, the driving compartment speedometer shall register when the generator drive system is engaged.

Where the generator is driven by the chassis engine and transmission through a split shaft PTO and a chassis transmission retarder is furnished, it shall be automatically disengaged for generator operations.

The direct drive generator shall be mounted so that it does not change the ramp break-over angle, angle of departure, or angle of approach as defined by other components, and it shall not extend into the ground clearance area.

The direct drive generator shall be mounted away from exhaust and muffler areas or provided with a heat shield to reduce operating temperatures in the generator area.

### **GENERATOR BONDING**

A minimum of four (4) 16" x 2 gauge copper ground straps shall be bolted to body sub-frame and chassis sub-frame for proper bonding of high voltage system. The conductor shall have a minimum amperage rating, as defined in 310.15, "Ampacities for Conductors Rated 0–2000 Volts," of *NFPA 70*, of 115 percent of the rated amperage on the power source specification label.

### **GENERATOR ENGAGEMENT**

A "Generator Engaged" indicator shall be provided in the driving compartment to indicate that the generator shift has been successfully completed.

An "OK to Operate Generator" indicator shall be provided in the driving compartment to indicate that the generator is engaged (if not always engaged), the transmission is in the proper gear (if required, automatic transmissions only), and the parking brake is engaged (if applicable).

An interlock system shall be provided to prevent advancement of the engine speed in the driving compartment or at any operator's panel unless the parking brake is engaged, and the transmission is in neutral or the output of the transmission is correctly connected to a pump or generator instead of the drive wheels.

### **12-LEAD GENERATOR CONNECTED VOLTAGE**

The above generator shall be internally wired as 120/208V "Wye" as to provide 120V on any one of the three (3) load carrying conductors too the current carrying ground conductor or 208V between any combination of pairs of the load carrying conductors.

## **GENERATOR CONTROL**

The generator shall be engaged at the multiplex display(s) in the cab.

## **GENERATOR MOUNTING - LIMA MAC**

The generator shall be mounted between the chassis frame rails. The generator mounting brackets shall be fabricated using steel plate and/or tubing and powder coat primed and painted black. The generator mounting shall be bolted between and/or to the sides of the chassis frame rails and removable so that the generator can be lowered from under the apparatus for service if necessary. The generator case shall extend above the top edge of the chassis frame rails and requires additional subframe height for clearance. There shall also be an access panel added to the body floor above the generator (where possible) to allow for wiring box access for service.

## **POWER-TAKE-OFF GENERATOR DRIVE**

There shall be a "Hot Shift" power-take-off (PTO) installed on the transmission PTO opening of the chassis. The "Hot Shift" PTO is provided to allow the engagement of the PTO at higher engine RPM speeds. The PTO output shall be connected to the generator through hollow tube type driveline with heavy duty universals.

The engagement of the PTO shall be in the chassis cab with a rocker switch and red pilot light to note engagement of the PTO or via the V-Mux screen if so equipped.

The power supply to the PTO engagement control shall be wired to the parking brake and a neutral position transmission switch to prevent engagement unless the vehicle is stopped and transmission has been placed in neutral.

The installation of the engine, transmission, driven accessories (power takeoffs (PTO), etc.) shall meet the engine and transmission manufacturers' installation recommendations for the service intended.

Model part number shall be Chelsea 280 series.

## **ENGINE SPEED CONTROL**

An engine speed auxiliary control device (high idle switch or throttle) shall be installed to maintain a stable cycle output from generator when the apparatus is parked.

An interlock shall prevent the operation of the engine speed auxiliary control device unless the parking brake is engaged and the transmission is in neutral or park, or the parking brake is engaged and the engine is disengaged from the drive wheels.

The engine shall be prevented from regulating its own engine speed during times when engine rpm control is critical for consistent apparatus functions such as generator, water pump, or aerial operation.

## **LOADCENTER**

The loadcenter shall be an Eaton BR Series specifically designed for protection and distribution of AC line voltage such as lighting and small motor branch circuits. The loadcenter enclosure is made of 16 gauge galvanized sheet steel with a galvanized coating provided for corrosion protection. All trims used on BR loadcenters are chromate sealed and finished with an electro-disposition epoxy paint (ANSI-61) which exceeds requirements for outdoor and indoor applications. A combination surface/flush cover with integral door is supplied with indoor loadcenters rated from 100 through 400 amperes. All plug-in loadcenters are CSA listed to file LL98266. CSA Certified to C22.2 No.29, to loadcenter type and CSA listing.

## **GENERATOR MONITORING PANEL**

An Accuenergy Acuvim II multifunction power and energy meter shall be provided to properly monitor the generator performance and load demand during operation. The Accuenergy Acuvim CL includes a digital RS485 communication port running Modbus protocol. The electrical parameters can be viewed on a backlit LCD screen. Unit shall be capable of displaying the following;

- Generator frequency in hertz
- Line voltage, phase to neutral or phase to phase, in volts
- Line current in amperes
- Meter running time

## **SHORE POWER INLET - BATTERY CHARGER**

The above mentioned shore power inlet, and battery conditioner shall be specified in the 12 volt section.

## **LINE VOLTAGE ELECTRICAL SYSTEM**

### **GENERAL REQUIREMENTS**

#### **Stability**

Any fixed line voltage power source producing alternating current (ac) shall produce electric power at 60 Hz,  $\pm 3$  Hz when producing power at all levels between no load and full rated power. Any fixed line voltage power source shall produce electric power at the rated voltage  $\pm 10$  percent when producing power at all levels between no load and full rated power.

The maximum voltage supplied to portable equipment shall not exceed 275 volts to ground. Higher voltage shall be permitted only when used to operate fixed wired, permanently mounted equipment on the apparatus.

#### **Conformance with National Electrical Code**

All components, equipment, and installation procedures shall conform to *NFPA 70, National Electrical Code*, except where superseded by the requirements of this chapter. Where the requirements of this chapter differ from those in *NFPA 70*, the requirements in this chapter shall apply.

Where available, line voltage electrical system equipment and materials included on the apparatus shall be listed and used only in the manner for which they have been listed. All equipment and materials shall be installed in accordance with the manufacturer's instructions.



### Location Ratings

Any equipment used in a dry location shall be listed for dry locations. Any equipment used in a wet location shall be listed for wet locations.

Any equipment, except a PTO-driven generator, used in an underbody or under chassis location that is subject to road spray shall be either listed as Type 4 or mounted in an enclosure that is listed as Type 4.

If a PTO-driven generator is located in an underbody or under chassis location, the installation shall include a shield to prevent road spray from splashing directly on the generator.

### Grounding

Grounding shall be in accordance with 250.34(A) and 250.34(B) of *NFPA 70*. Ungrounded systems shall not be used.

Only stranded or braided copper conductors shall be used for grounding and bonding.

The grounded current-carrying conductor (neutral) shall be insulated from the equipment-grounding conductors and from the equipment enclosures and other grounded parts.

The neutral conductor shall be colored white or gray in accordance with 200.6, "Means of Identifying Grounded Conductors," of *NFPA 70*.

Any bonding screws, straps, or buses in the distribution panel board or in other system components between the neutral and equipment-grounding conductor shall be removed and discarded.

### Bonding

The neutral conductor of the power source shall be bonded to the vehicle frame. The neutral bonding connection shall occur only at the power source. In addition to the bonding required for the low voltage return current, each body and each driving or crew compartment enclosure shall be bonded to the vehicle frame by a copper conductor.

The conductor shall have a minimum ampere rating, as defined in 310.15, "Ampacities for Conductors Rated 0–2000 Volts," of *NFPA 70*, of 115 percent of the rated ampere on the power source specification label.

A single conductor that is sized to meet the low voltage and line voltage requirements shall be permitted to be used.

### Ground Fault Circuit Interrupters

In special service vehicles incorporating a lavatory, sink, toilet, shower, or tub, 120 V, 15 or 20 A receptacles within 6 ft (1.8 m) of these fixtures shall have ground fault circuit interrupter (GFCI) protection. GFCIs integrated into outlets or circuit breakers or as stand-alone devices shall be permitted to be used in situations.

### Power Source General Requirements

All power source system mechanical and electrical components shall be sized to support the continuous duty nameplate rating of the power source.

The power source shall be shielded from contamination that would prevent the power source from operating within its design specifications.

### Power Source Rating

For power sources of 8 kW or larger, the power source manufacturer shall declare the continuous duty rating that the power source can provide when installed on fire apparatus according to the manufacturer's instructions and run at 120°F (49°C) air intake temperature at 2000 ft (600 m) above sea level.

The rating on the power source specification label shall not exceed the declared rating from the power source manufacturer.

Access shall be provided to permit both routine maintenance and removal of the power source for major servicing. The power source shall be located such that neither it nor its mounting brackets interfere with the routine maintenance of the fire apparatus.

### Instrumentation

If the power source is rated at less than 3 kW, a “Power On” indicator shall be provided. If the power source is rated at 3 kW or more but less than 8 kW, a voltmeter shall be provided.

If the power source is rated at 8 kW or more, the following instrumentation shall be provided at an operator’s panel:

- 1) Voltmeter
- 2) Current meters for each ungrounded leg
- 3) Frequency (Hz) meter
- 4) Power source hour meter

The instrumentation shall be permanently mounted at an operator’s panel. The instruments shall be located in a plane facing the operator. Gauges, switches, or other instruments on this panel shall each have a label to indicate their function.

The instruments and other line voltage equipment and controls shall be protected from mechanical damage and not obstructed by tool mounting or equipment storage.

An instruction plate(s) that provides the operator with the essential power source operating instructions, including the power-up and power-down sequence, shall be permanently attached to the apparatus at any point where such operations can take place.

### Operation

Provisions shall be made for placing the generator drive system in operation using controls and switches that are identified and within convenient reach of the operator.

Where the generator is driven by the chassis engine and engine compression brakes or engine exhaust brakes are furnished, they shall be automatically disengaged for generator operations.

Any control device used in the generator system power train between the engine and the generator shall be equipped with a means to prevent unintentional movement of the control device from its set position in the power generation mode.

If there is permanent wiring on the apparatus that is designed to be connected to the power source, a power source specification label that is permanently attached to the apparatus at the operator’s control station shall provide the operator with the information required.

The power source, at any load, shall not produce a noise level that exceeds 90 dBA in any driving compartment, crew compartment, or onboard command area with windows and doors closed or at any operator’s station on the apparatus.

### Power Supply Assembly

The conductors used in the power supply assembly between the output terminals of the power source and the main over current protection device shall not exceed 12 ft (4 m) in length.

All power supply assembly conductors, including neutral and grounding conductors, shall have an equivalent amperage rating and shall be sized to carry not less than 115 percent of the amperage of the nameplate current rating of the power source.

If the power supply assembly connects to the vibrating part of a generator (not a connection on the base), the conductors shall be flexible cord or other fine-stranded conductors enclosed in metallic or nonmetallic liquid tight flexible conduit rated for wet locations and temperatures not less than 194°F (90°C).

### Over-current Protection

Manually re-settable over current devices shall be installed to protect the line voltage electrical system components.

### Power Source Protection

A main over current protection device shall be provided that is either incorporated in the power source or connected to the power source by a power supply assembly.

The size of the main over current protection device shall not exceed 100 percent of the rated amperage stated on the power source specification label or the rating of the next larger available size over current protection device, where so recommended by the power source manufacturer.

If the main over current protection device is subject to road spray, the unit shall be housed in a Type 4-rated enclosure.

### Branch Circuit Over-current Protection

Over current protection devices shall be provided for each individual circuit and shall be sized at not less than 15 amps in accordance with 240.4, "Protection of Conductors," of *NFPA 70*.

Any panel board shall have a main breaker where the panel has six or more individual branch circuits or the power source is rated 8 kW or larger.

Each over current protection device shall be marked with a label to identify the function of the circuit it protects.

Dedicated circuits shall be provided for any large appliance or device (air conditioning units, large motors, etc.) that requires 60 percent or more of the rated capacity of the circuit to which it is connected, and that circuit shall serve no other purpose.

### Panelboards

All fixed power sources shall be hardwired to a permanently mounted panel board unless one of the following conditions exists:

- 1) All line voltage power connections are made through receptacles on the power source and the receptacles are protected by integrated over current devices.
- 2) Only one circuit is hardwired to the power source, which is protected by an integrated over current device.

The panel shall be visible and located so that there is unimpeded access to the panel board controls. All panel boards shall be designed for use in their intended location. The panel(s) shall be protected from mechanical damage, tool mounting, and equipment storage.

Where the power source is 120/240 V and 120 V loads are connected, the apparatus manufacturer or line voltage system installer shall consider load balancing to the extent that it is possible.

### Wiring Methods

Fixed wiring systems shall be limited to the following:

- 1) Metallic or nonmetallic liquid tight flexible conduit rated at temperatures not less than 194°F (90°C) with stranded copper wire rated for wet locations and temperatures not less than 194°F (90°C)
- 2) Type SOW, SOOW, SEOW, or SEOOW flexible cord rated at 600 V and at temperatures not less than 194°F (90°C)

Electrical cord or conduit shall not be attached to chassis suspension components, water or fuel lines, air or air brake lines, fire pump piping, hydraulic lines, exhaust system components, or low voltage wiring and shall be arranged as follows:

- 1) Separated by a minimum distance of 12 in. (300 mm) from exhaust piping or shielded from such piping
- 2) Separated from fuel lines by a minimum distance of 6 in. (150 mm)

A means shall be provided to allow “flexing” between the driving and crew compartment, the body, and other areas or equipment whose movement would stress the wiring.

Electrical cord or conduit shall be supported within 6 in. (150 mm) of any junction box and at a minimum of every 24 in. (600 mm) of run.

Supports shall be made of nonmetallic materials or of corrosion-resistant or corrosion-protected metal. All supports shall be of a design that does not cut or abrade the conduit or cord and shall be mechanically fastened to the apparatus.

Only fittings and components listed for the type of cord or conduit being installed shall be used.

Splices shall be made only in a listed junction box.

### Additional Requirements for Flexible Cord Installations

Where flexible cord is used in any location where it could be damaged, it shall be protected by installation in conduit, enclosures, or guards.

Where flexible cord penetrates a metal surface, rubber or plastic grommets or bushings shall be installed.

### Wiring Identification

Each line voltage circuit originating from the main panel board shall be identified.

The wire or circuit identification either shall reference a wiring diagram or wire list or shall indicate the final termination point of the circuit.

Where pre-wiring for future power sources or devices exists, the un-terminated ends shall be marked with a label showing their wire size and intended function.

### Wiring System Components

Only stranded copper conductors with an insulation rated for temperatures of at least 194°F (90°C) and wet locations shall be used. Conductors in flexible cord shall be sized in accordance with Table 400.5(A) of *NFPA 70*. Conductors used in conduit shall be sized in accordance with 310.15, "Ampacities for Conductors Rated 0–2000 Volts," of *NFPA 70*. Aluminum or copper-clad aluminum conductors shall not be used.

All boxes shall conform to and be mounted in accordance with Article 314, "Outlet, Device, Pull, and Junction Boxes; Conduit Bodies; Fittings; and Manholes," of *NFPA 70*. All boxes shall be accessible using ordinary hand tools. Boxes shall not be permitted behind welded or pop-riveted panels.

The maximum number of conductors permitted in any box shall be in accordance with 314.16, "Number of Conductors in Outlet, Device, and Junction Boxes, and Conduit Bodies," of *NFPA 70*.

All wiring connections and terminations shall provide a positive mechanical and electrical connection. Connectors shall be installed in accordance with the manufacturer's instructions. Wire nuts or insulation displacement and insulation piercing connectors shall not be used.

Each switch shall indicate the position of its contact points (i.e., open or closed) and shall be rated for the continuous operation of the load being controlled. All switches shall be marked with a label indicating the function of the switch. Circuit breakers used as switches shall be "switch rated" (SWD) or better. Switches shall simultaneously open all associated line voltage conductors. Switching of the neutral conductor alone shall not be permitted.

Line voltage circuits controlled by low voltage circuits shall be wired through properly rated relays in listed enclosures that control all non-grounded current-carrying conductors.

### Receptacles and Inlet Devices

#### Wet and Dry Locations

All wet location receptacle outlets and inlet devices, including those on hardwired, remote power distribution boxes, shall be of the grounding type, provided with a wet location cover, and installed in accordance with Section 406.8, "Receptacles in Damp or Wet Locations," of *NFPA 70*.

All receptacles located in a wet location shall be not less than 24 in. (600 mm) from the ground. Receptacles on off road fire apparatus shall be a minimum of 30 in. (750 mm) from the ground. All receptacles located in a dry location shall be of the grounding type and shall be at least 12 in. (300 mm) above the interior floor height. No receptacle shall be installed in a face-up position.

The face of any wet location receptacle shall be installed in a plane from vertical to not more than 45 degrees off vertical.

#### Receptacle Label

Each receptacle shall be marked with a label indicating the nominal line voltage (120 volts or 240 volts) and the current rating in amps of the circuit. If the receptacle is DC or other than single phase, that information shall also be marked on the label.

All receptacles and electrical inlet devices shall be listed to UL 498, *Standard for Safety Attachment Plugs and Receptacles*, or other recognized performance standards.

Receptacles used for DC voltages shall be rated for DC service.

### Wiring Schematics

An "As-Built" Wiring diagrams for line voltage systems shall be provided to include the following information;

- (a) Pictorial representations of circuit logic for all electrical components and wiring
- (b) Circuit identification
- (c) Connector pin identification
- (d) Zone location of electrical components
- (e) Safety interlocks
- (f) Alternator–battery power distribution circuits
- (g) Input/output assignment sheets or equivalent circuit logic implemented in multiplexing systems

### **LIGHT TOWER**

One (1) Command Light, CL Series light tower(s) shall be provided and installed on the completed unit.

The Command Light shall be covered by a five (5) year limited warranty from defects in materials and workmanship. An operation, maintenance, and parts manual shall be provided with the completed unit.

#### Light Tower Construction and Design

The Command Light assembly shall be of aluminum construction, with stainless steel shafts and bronze bushings for long life and low maintenance.

The electrically controlled unit shall not require usage of the vehicle's air supply for operation, thereby eliminating the chance for air leaks in the vehicle braking system. Hydraulic or pneumatic type floodlights are not acceptable alternatives to the specified all electric light tower.

The light tower shall be tested to in wind conditions of 90 mph (150 kph) minimum. Light towers that have not been tested to these conditions are not acceptable.

The light tower shall be capable of overhanging the side or back of the vehicle to provide maximum illumination to the vicinity adjacent to the vehicle for the safety of emergency personnel in high traffic conditions. Light towers that are only capable of rotation at the top of a pole are not acceptable to the specified light tower.

#### Light Tower Electrical System

The light tower shall be a two-stage articulating device with a lighting bank on top of the second stage capable of continuous 360 degree rotation. The light shall be elevated by electric linear actuators, one (1) actuator shall elevate the light bank and one (1) actuator shall adjust the light bank angle from 0 to 110 degrees. Power for the light bank shall be supplied through power collecting rings thus allowing continuous 360 degree rotation in either direction.

The tower base shall have a light that illuminates the envelope of motion during any movement of the light tower mast as required by NFPA 1901.

A red flashing or rotating light located in the driving compartment shall be illuminated automatically whenever the vehicles parking brake is not fully engaged, indicating that the light tower is not in stowed position, as required by NFPA 1901.

### Light Tower Floodlights

The Command Light model CL802A-CH shall be equipped with the following bank of floodlights:

Floodlight manufacturer:	Fire Tech
Number of lamp heads:	Eight (8) Helios LED
Voltage:	120 volts
Watts of each lamp head:	60 watt
Total watts of light tower:	780 watts
Total lumens of light tower:	112,000 lumens
Configuration:	The light heads shall be mounted with four (4) on each side of the light tower, giving two (2) vertical lines of four (4) when the lights are in the upright position.

### Light Tower Backlight Option

A backlight option shall be provided on the light tower. The lower two (2) pair of light heads shall be capable of being rotated about a horizontal axis 180 degree, providing light down on the vehicle or to the opposite side of the vehicle while allowing the fixed lights to remain pointed at the scene.

The hand-held remote control shall have an additional switch supplied for the backlight rotation option.

### Light Tower Paint

The light tower shall be electro-statically powder coated with a hammer tone gray color.

### Light Tower Controls

The light tower(s) shall be operated with a hand-held 15-foot umbilical line remote control. The storage station for the remote control unit shall be equipped with a button to activate the "Auto-Park" automatic nesting feature. The remote control shall be located per the itemized compartment list and include;

Three (3) switches; one (1) for each pair of lights.

One (1) switch for light bank rotation.

One (1) switch for elevating lower stage.

One (1) switch for elevating upper stage.

One (1) switch for optional light bank rotation.

One (1) switch for the optional strobe.

One (1) indicator light to indicate when light bank is out of the roof nesting position.

One (1) indicator light to indicate when light bank is rotated to proper nesting position.

### Light Tower Mounting

The specified light tower(s) shall be mounted on the roof of the body.

Where the light tower is to be mounted above a finished walk-in area; the roof backing plates and structure shall have threaded holes to allow removal of light tower without removal of the interior paneling.

Where the light tower is mounted in close proximity to other roof mounted items (i.e. antennas, air conditioners, and weather stations) the light tower shall be orientated in order to help prevent a operator driven collision.



## **EQUIPMENT PAYLOAD WEIGHT ALLOWANCE**

In compliance with NFPA 1901 standards, the special service vehicle shall be designed for an equipment loading allowance of 6,000 lbs. of Riverside County Fire Department provided equipment based on a 40,001 - 50,000 pound gross vehicle weight rating.

## **EQUIPMENT**

The following equipment shall be furnished with the completed special service vehicle;

- One (1) container of assorted stainless steel nuts, bolts, screws and washers used in the construction of the apparatus shall be provided with the completed apparatus.
- Four (4) PAC Toolok model 1003HD bracket(s) with black strap shall be provided with the completed vehicle.

Brackets to be installed in S4 Compartment aft wall for customer supplied 6' Rubbish hook and 6' NY Roof hook

- There shall be two (2) Zico SAC-44-E NFPA approved folding aluminum wheel chocks provided for 44" diameter tires that together will hold the vehicle when loaded to its GVWR or GCWR, on a hard surface with a 20 % grade, with the transmission in neutral, and the parking brake released.
  - The wheel chock(s) shall be shipped loose with the completed apparatus.
- One (1) 20 lb. ABC dry chemical aluminum fire extinguisher(s) shall be provided with the completed unit.
  - The above specified fire extinguisher(s) shall be installed on the completed unit, location to be **in S4 or S3 where it will fit. (review in 3D screen shots)**
- One (1) 2-1/2 gallon pressurized water (Class A) fire extinguisher(s) shall be provided with the completed unit.

The above specified fire extinguisher(s) shall be installed on the completed unit, location to be **in S4 or S3 where it will fit. (review in 3D screen shots)**

- **Four (4) Yellow Pelican 9440 Remote Area Lights**  
Will be stored in S2 top shelf.

The 9440 now offers three pre-set power levels, battery level indication and comes equipped with a lithium ion rechargeable battery. The 9440 moves fast to light up ravines, confined spaces, riverbanks, anyplace generator lights can't go. Deployed, the mast extends 7 feet (2.1 meters) high, shining light over low obstructions encountered by traditional lantern style lights. With a 125 degree beam spread and up to 5300 lumens, your entire work area will have the light you need for a safe and efficient operation. The 9440 is able to run directly from wall power if needed and can be left on charge indefinitely which makes for an invaluable emergency preparedness tool.

The 9440 is maintenance free, using super tough LED lamp modules and a lithium ion battery for up to 8 hours of continuous light.

Adjustable carrying strap included.

- Up to 5300 lumens
- Up to 8 hours run time
- Mast extends 7 feet (2.1 meters) high when deployed
- Convenient shoulder strap
- Equipped with a lithium ion rechargeable battery
- Built Pelican tough
- RoHS and CE Compliant
- Two (2) Streamlight Fire Vulcan C4 LED flashlight(s) with shoulder strap shall be provided with 80,000 candela and 3 hour run time. Each flashlight shall be orange in color and have a 12 volt DC charger and vehicle mount kit. Each flashlight shall have an LED spotlight style bulbs and reflectors. The flashlight(s) shall be wired to battery direct unless otherwise specified by Riverside County Fire Department.

**Will be model # 44451**

- Two (2) flashlight(s) shall be mounted on the completed unit in the compartment **S4**.

#### **REMAINING NFPA MINOR EQUIPMENT BY PURCHASER**

All other minor equipment not specified above, but required by NFPA 1901 for special service vehicles, section 10.9.3 shall be supplied and mounted by Riverside County Fire Department before the unit is placed in emergency service.